

Fig. 5 Variations in tube voltage and current with charging voltages of (a) -50 kV, (b) -60 kV, and (c) -70 kV.

current transformer, respectively (Fig. 5). The voltage and current displayed roughly damped oscillations, because the discharge resistance in the tube varied rapidly from infinity to approximately 0Ω during the discharge. Thus, at the first quarter cycle of the oscillations, when the voltage decreased, the current increased. Within twice the potential of the condenser charging voltage, the instantaneous voltage increases according to increases in the charging voltage and

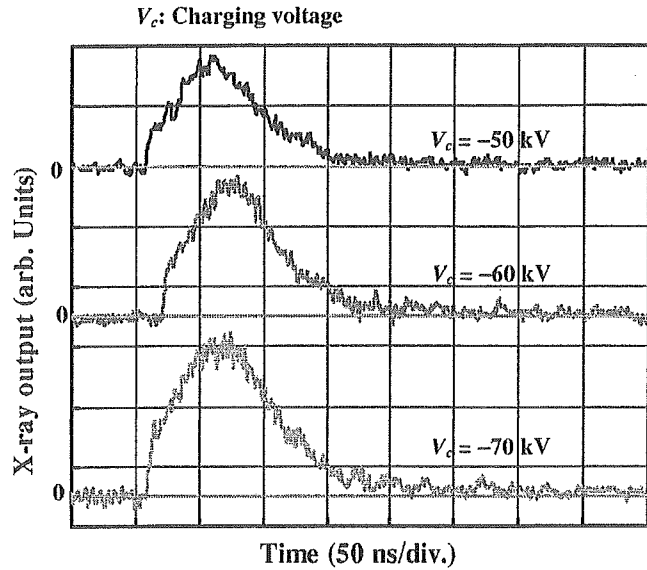


Fig. 6 X-ray outputs at the indicated conditions using the filter.

to increases in the target-cathode space. On the other hand, the instantaneous current increases with increases in the charging voltage and decreases in the space. At a space of 1.0 mm, the instantaneous voltage and current increased with increases in the charging voltage, and the voltage and current were approximately 90 kV and 0.8 kA, respectively, at a charging voltage of -70 kV.

3.2 X-ray Output

An x-ray output pulse was detected using a combination of a plastic scintillator, a photomultiplier, and the filter (Fig. 6). When the charging voltage was increased, the pulse height increased, but the width seldom varied. The widths were approximately 80 ns, and the time-integrated x-ray dose measured using a thermoluminescence dosimeter (Kyokko TLD Reader 1500 having MSO-S elements without energy compensation) had a value of approximately $90 \mu\text{Gy}$ per pulse at 0.3 m from the x-ray source with a charging voltage of -70 kV. In the dose measurement, five elements (detectors) with a diameter of 2.0 mm and a length of 11 mm were set at 0.3 m from the x-ray source, and the dose was the average value of ten shots of flash

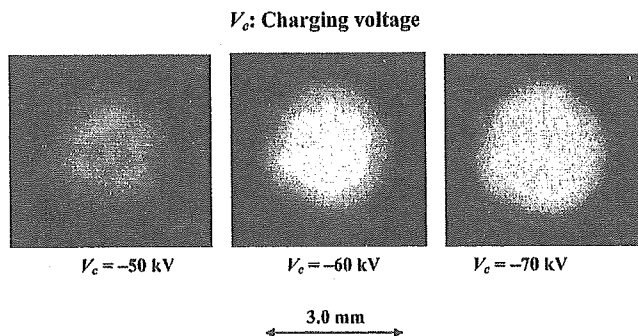


Fig. 7 Images of x-ray sources of $K\alpha$ lines with changes in the charging voltage.

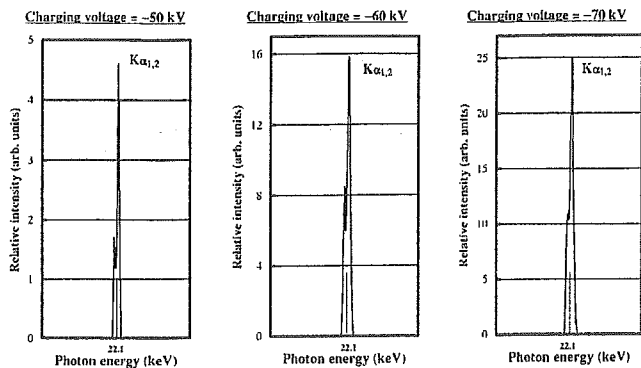


Fig. 8 X-ray spectra from a silver target with the filter.

x-rays and five elements. Using this high-voltage pulse generator, the maximum repetition rate of flash x-rays was approximately 50 Hz. At a charging voltage of -70 kV and the maximum rate, the electric power of the flash x-ray generator and the dose rate are estimated at approximately 200 W and 400 $\mu\text{Gy/s}$ at 1.0 m, respectively.

3.3 X-ray Source

To observe the x-ray source, we employed a 100- μm -diam pinhole camera, an x-ray film (Polaroid XR-7), and the filter (Fig. 7). When the charging voltage was increased, the spot intensity increased, and the intensities corresponded well to the x-ray pulse height. The dimension was almost equal to the target diameter and had a value of approximately 3.0 mm.

3.4 X-ray Spectra

X-ray spectra were measured by a transmission-type spectrometer with a lithium fluoride curved crystal 0.5 mm thick. The spectra were taken using a computed radiography (CR) system¹⁸ (Konica Regius 150) with a wide dynamic range, and relative x-ray intensity was calculated from Dicom digital data. Figure 8 shows the measured spectra from the silver target with the filter. We observed clean $K\alpha$ lines, while bremsstrahlung rays were hardly de-

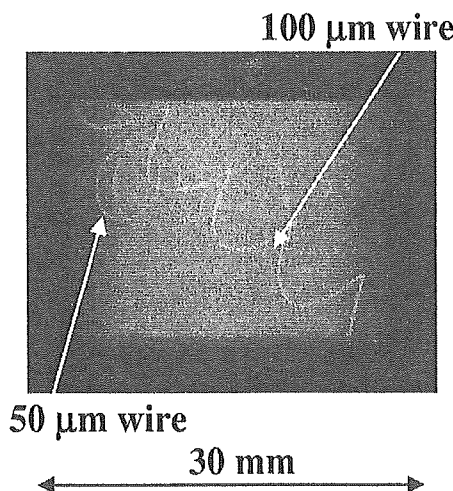


Fig. 9 Radiograms of tungsten wires of 50 and 100 μm in a rod made of polymethyl methacrylate.

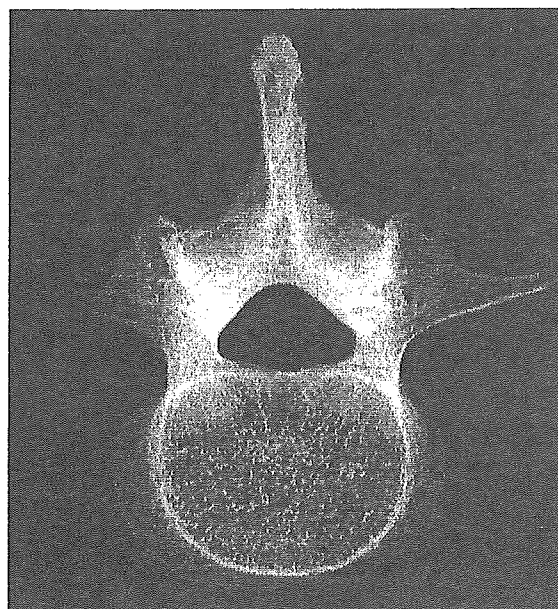


Fig. 10 Radiogram of a vertebra.

ected. When the charging voltage was increased, the instantaneous tube voltage and current increased, and the $K\alpha$ intensity substantially increased.

3.5 Radiography

Monochromatic flash radiography was performed using the CR system 0.3 m from the x-ray source with the filter, and the charging voltage was -70 kV. First, rough measure-

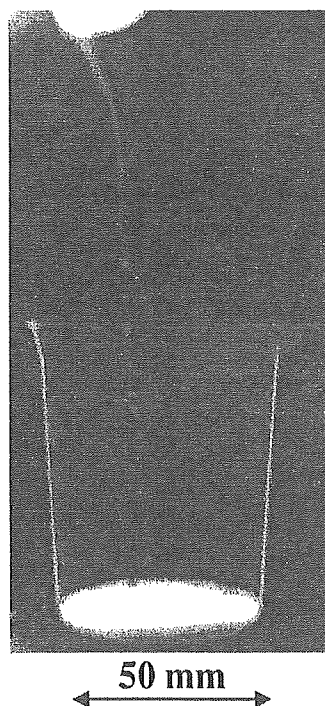


Fig. 11 Radiogram of water falling into a polypropylene beaker from a glass test tube.

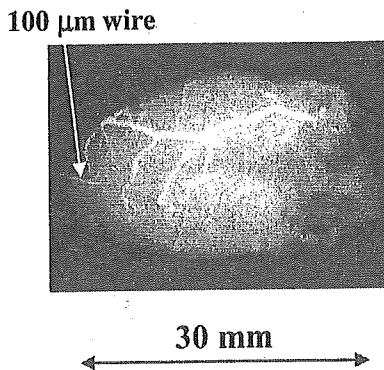


Fig. 12 Angiogram of a rabbit heart.

ments of spatial resolution were made using wires. Figure 9 shows radiograms of tungsten wires in a rod made of polymethyl methacrylate. Although the image contrast increased with increases in the wire diameter, a 50- μm -diam wire could be observed.

Figure 10 shows a radiogram of a vertebra, and fine structures in the vertebra are observed. Next, the image of water falling into a polypropylene beaker from an injector is shown in Fig. 11. This image was taken with the slight addition of an iodine-based contrast medium. Because the x-ray duration was approximately 80 ns, the stop-motion image of water could be obtained. Figure 12 shows an angiogram of a rabbit heart; iodine-based microspheres 15 μm in diameter were used, and fine blood vessels of approximately 100 μm were visible.

4 Conclusion and Outlook

Concerning the spectrum measurement, we obtained fairly clean silver $K\alpha$ rays (22.1 keV). Therefore, we are very interested in the measurement of the $K\alpha$ rays from cerium (34.6 keV) and tungsten (58.9 keV) targets. The target element should be selected corresponding to the radiographic objectives. In medical applications, K-series characteristic x-rays of cerium are absorbed effectively by an iodine-based contrast medium with a K-edge of 33.2 keV, and K-edge angiography can be performed.

In this research, the instantaneous number of generator-produced $K\alpha$ photons was approximately 4×10^7 photons/cm² per pulse 0.3 m from the source. However, the intensity can be increased by increasing the electrostatic energy in condensers in the surge generator, and quasimonochromatic x-rays of both $K\alpha$ and $K\beta$ (24.9 keV) lines are produced without using the palladium filter with a K-edge of 24.3 keV.

Using this flash x-ray generator, because the photon energy of characteristic x-rays can be selected, a high-speed photon-counting radiography system can be performed to decrease noise from radiograms. As compared with a steady state x-ray generator, since the target element can be changed easily using this demountable PMMA tube, demonstrations of monochromatic radiography will be accomplished easily.

Acknowledgment

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, and 16591222) and Advanced Medical Scientific Research from MECSSST, Health and Labor Sciences Research Grants (RAMT-nano-001, RHGTEFB-genome-005, and RHGTEFB-saisei-003), grants from the Keiryō Research Foundation, the Promotion and Mutual Aid Corporation for Private Schools of Japan, Japan Science and Technology Agency (JST), and New Energy and Industrial Technology Development Organization (NEDO, Industrial Technology Research Grant Program in 2003).

References

1. A. C. Thompson, H. D. Zeman, G. S. Brown, J. Morrison, P. Reiser, V. Padmanabahn, L. Ong, S. Green, J. Giacomini, H. Gordon, and E. Rubenstein, "First operation of the medical research facility at the NSLS for coronary angiography," *Rev. Sci. Instrum.* **63**, 625–628 (1992).
2. H. Mori, K. Hyodo, E. Tanaka, M. U. Mohammed, A. Yamakawa, Y. Shinozaki, H. Nakazawa, Y. Tanaka, T. Sekka, Y. Iwata, S. Honda, K. Umetani, H. Ueki, T. Yokoyama, K. Tanioka, M. Kubota, H. Hosaka, N. Ishizawa, and M. Ando, "Small-vessel radiography in situ with monochromatic synchrotron radiation," *Radiology* **201**, 173–177 (1996).
3. K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita, and J. Tada, "Development of a two-dimensional imaging system for clinical applications of intravenous coronary angiography using intense synchrotron radiation produced by a multipole wiggler," *J. Synchrotron Radiat.* **5**, 1123–1126 (1998).
4. E. Sato, S. Kimura, S. Kawasaki, H. Isobe, K. Takahashi, Y. Tamakawa, and T. Yanagisawa, "Repetitive flash x-ray generator utilizing a simple diode with a new type of energy-selective function," *Rev. Sci. Instrum.* **61**, 2343–2348 (1990).
5. E. Sato, M. Sagae, K. Takahashi, T. Oizumi, H. Ojima, K. Takayama, Y. Tamakawa, T. Yanagisawa, A. Fujiwara, and K. Mitoya, "High-speed soft x-ray generators in biomedicine," *Proc. SPIE* **2513**, 649–667 (1994).
6. E. Sato, M. Sagae, K. Takahashi, A. Shikoda, T. Oizumi, H. Ojima, K. Takayama, Y. Tamakawa, T. Yanagisawa, A. Fujiwara, and K. Mitoya, "Dual energy flash x-ray generator," *Proc. SPIE* **2513**, 723–735 (1994).
7. A. Shikoda, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa, and T. Yanagisawa, "Repetitive flash x-ray generator having a high-durability diode driven by a two-cable-type line pulser," *Rev. Sci. Instrum.* **65**, 850–856 (1994).
8. E. Sato, K. Takahashi, M. Sagae, S. Kimura, T. Oizumi, Y. Hayasi, Y. Tamakawa, and T. Yanagisawa, "Sub-kilohertz flash x-ray generator utilizing a glass-enclosed cold-cathode triode," *Med. Biol. Eng. Comput.* **32**, 289–294 (1994).
9. K. Takahashi, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa, and T. Yanagisawa, "Fundamental study on a long-duration flash x-ray generator with a surface-discharge triode," *Jpn. J. Appl. Phys., Part 1* **33**, 4146–4151 (1994).
10. E. Sato, Y. Hayasi, E. Tanaka, H. Mori, T. Kawai, T. Usuki, K. Sato, H. Obara, T. Ichimaru, K. Takayama, H. Ido, and Y. Tamakawa, "Quasi-monochromatic radiography using a high-intensity quasi-x-ray laser generator," *Proc. SPIE* **4682**, 538–548 (2002).
11. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, H. Obara, T. Ichimaru, K. Takayama, and H. Ido, "Intense characteristic x-ray irradiation from weakly ionized linear plasma and applications," *Jpn. J. Med. Imag. Inform. Sci.* **20**, 148–155 (2003).
12. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, H. Obara, T. Ichimaru, K. Takayama, and H. Ido, "Irradiation of intense characteristic x-rays from weakly ionized linear molybdenum plasma," *Jpn. J. Med. Phys.* **23**, 123–131 (2003).
13. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama, and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing weakly ionized linear copper plasma," *Rev. Sci. Instrum.* **74**, 5236–5240 (2003).
14. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama, and H. Ido, "Sharp characteristic x-ray irradiation from weakly ionized linear plasma," *J. Electron Spectrosc. Relat. Phenom.* **137–140**, 713–720 (2004).
15. A. Mattsson, "Some characteristics of a 600 kV flash x-ray tube," *Phys. Scr.* **5**, 99–102 (1972).
16. R. Germer, "X-ray flash techniques," *J. Phys. E* **12**, 336–350 (1979).
17. B. K. Agarwal, *X-Ray Spectroscopy*, 2nd ed., p. 18, Springer-Verlag, New York (1991).

18. E. Sato, K. Sato, and Y. Tamakawa, "Film-less computed radiography system for high-speed Imaging," *Ann. Rep. Iwate Med. Univ. Sch. Lib. Arts Sci.* **35**, 13–23 (2000).

Eiichi Sato received his BS, MS, and PhD in applied physics from Tohoku Gakuin University, Sendai, Japan, in 1979, 1982, and 1987, respectively. He is currently a professor in the Department of Physics at Iwate Medical University. He has written approximately 400 publications and delivered some 200 international presentations concerning x-rays. His research interests include soft flash x-ray generators, quasi-x-ray laser generators, and high-speed radiography. In 2000, he received the Schardin Gold Medal from the German Physical Society, in 2003 he received the Takayama Award (Gold Medal) from the Japan Society of High Speed Photography and Photonics, and he received the Honorable Mention Poster Award from the SPIE International Symposium on Medical Imaging 2005.

Yasuomi Hayasi received his BS, MS, and PhD degrees in physics from Tohoku University in 1962, 1964, and 1967, respectively. Since 1990 he has been a professor in the Department of Electrical Engineering at Hachinohe National College of Technology, Japan. Since 2003 he has been a visiting professor at the Department of Physics, Iwate Medical University. His research interests include x-ray spectroscopy.

Rudolf Germer received his diploma, PhD, and habile degrees in physics in 1971, 1974, and 1979 at the Free and Technical Universities of Berlin. He was a visiting professor at the University of Oldenburg (Germany) and ODU Norfolk, and did research at the Fritz-Haber Institute (MPI Berlin). He was professor at the University of Applied Science Telekom Berlin and is now at the FHTW and TU Berlin. He is president of the Institute of Technical Physics e.V. His research interests include areas of technical physics such as x-ray flashes, pulsed power, solid state and plasma physics, sound, and high-speed videography. He received the High-Speed Imaging Award 2003 of Japan.

Etsuro Tanaka received his MD and PhD degrees in medicine from Kumamoto University, Japan, in 1980 and 1986, respectively. He worked on medical image processing in the Department of Physiology, Tokai University, Japan, from 1988 to 2003. He is currently a professor in the Department of Nutritional Sciences, Tokyo University of Agriculture, Japan. His research interests include medical image processing, human physiology, and clinical nutrition.

Hidezo Mori received a medical degree from Keio University School of Medicine, Tokyo, Japan, in 1977, and also a PhD from the Post Graduate School, Keio University School of Medicine. Now he is the director of the Department of Cardiac Physiology at the National Cardiovascular Center, Suita, Japan. His primary research interests are regenerative therapy in cardiovascular disease, microcirculation, and medical applications of structural biology.

Toshiaki Kawai received the BS degree in precision mechanics and the MS degree in electronic engineering from Shizuoka University, Hamamatsu, Japan in 1964 and 1974, respectively. In 1974, he joined the Hamamatsu Photonics K.K., where he worked on research and development of solid-state infrared detectors. From 1978 to 1981, he engaged in research work on the NEA cold cathode for application to imaging camera tubes. He is now the project coordinator of the Electron Tube Division 2 and is engaged in the development and manufacturing of imaging devices and x-ray equipment. He is a member of the Japan Radioisotope Association and the Institute of Image Information and Television Engineers of Japan.

Takashi Inoue received his MD and PhD degrees in 2000 from Tohoku University. He is currently an assistant professor in the Department of Neurosurgery at Iwate Medical University, and a member of the Japan Neurosurgical Society. His research interests include neurosurgery and MRI.

Akira Ogawa received his MD and PhD degrees in 1981 from Tohoku University. He is currently a professor in the Department of Neurosurgery and Dean of the School of Medicine at Iwate Medical University, and is a trustee of the Japan Neurosurgical Society. His research interests include neurosurgery and cerebrovascular disease.

Shigehiro Sato received his MD degree from Iwate Medical University in 1980. He worked for the laboratory of the Division of Pediatric Infectious Diseases at Johns Hopkins Hospital from 1985 to 1989. He is currently a professor in the Department of Microbiology at Iwate Medical University. His research interests include central nervous system damage caused by Vero toxin, a cell culture system for vaccine development, and microangiography.

Toshio Ichimaru received his PhD degree in medical science in 1983 from Iwate Medical University. He is currently a professor of Medical Radiological Science, School of Health Sciences, at Hirosaki University. His research interests include various kinds of x-ray imaging in medicine.

Kazuyoshi Takayama received his BS degree from Nagoya Institute of Technology in 1962. In 1970, he received his PhD in mechanical engineering from Tohoku University. He is currently a director (professor) in the Shock Wave Research Center, Institute of Fluid Science at Tohoku University. His research interests include various shock wave phenomena, high-speed photography, and flash radiography. He has received seven awards including the coveted Ernst Mach Medal in 2000.

Jun Onagawa received his BS and PhD degrees in applied physics from Tohoku Gakuin University in 1968 and 2001, respectively. He is currently a professor in the Department of Applied Physics and Informatics, Faculty of Engineering at Tohoku Gakuin University. His research interests include target metallography and x-ray spectroscopy.

Hideaki Ido received his BS, MS, and PhD degrees in physics from Tohoku University in 1962, 1964, and 1967, respectively. He is currently a professor in the Department of Applied Physics and Informatics, Faculty of Engineering at Tohoku Gakuin University. His research interests include magnetism and x-ray spectroscopy.

X-ray spectra from a cerium target and their application to cone beam K-edge angiography

Eiichi Sato, MEMBER SPIE
Iwate Medical University
Department of Physics
Morioka 020-0015, Japan
E-mail: dresato@iwate-med.ac.jp

Akira Yamadera
Hirosaki University
Department of Radiological Technology
School of Health Sciences
Hirosaki 036-8564, Japan

Etsuro Tanaka
Tokyo University of Agriculture
Department of Nutritional Science
Faculty of Applied Bioscience
Setagaya-ku 156-8502, Japan

Hidezo Mori
National Cardiovascular Center Research Institute
Department of Cardiac Physiology
Osaka 565-8565, Japan

Toshiaki Kawai, MEMBER SPIE
Hamamatsu Photonics K. K.
Electron Tube Division 2
Iwata 438-0193, Japan

Fumihito Ito
Digital Culture Technology Corporation
Kanno The 2nd Building
Morioka 020-0021, Japan

Takashi Inoue
Akira Ogawa
Iwate Medical University
Department of Neurosurgery
School of Medicine
Morioka 020-8505, Japan

Shigehiro Sato
Iwate Medical University
Department of Microbiology
School of Medicine
Morioka 020-8505, Japan

Kazuyoshi Takayama, MEMBER SPIE
Tohoku University
Shock Wave Research Center
Institute of Fluid Science
Sendai 980-8577, Japan

Jun Onagawa
Hideaki Ido
Tohoku Gakuin University
Department of Applied Physics and Informatics
Faculty of Engineering
Tagajo 985-8537, Japan

Abstract. The cerium-target x-ray tube is useful for performing cone beam K-edge angiography, because K-series characteristic x-rays from the cerium target are absorbed effectively by iodine-based contrast media. The x-ray generator consists of a main controller and a unit with a high-voltage circuit and a fixed anode x-ray tube. The tube is a glass-enclosed diode with a cerium target and a 0.5-mm-thick beryllium window. The maximum tube voltage and current are 65 kV and 0.4 mA, respectively, and the focal-spot sizes are 1.3×0.9 mm. Cerium K-series characteristic x-rays are left, using a 3.0-mm-thick aluminum filter, and the x-ray intensity is $19.9 \mu\text{Gy/s}$ at 1.0 m from the source with a tube voltage of 60 kV and a current of 0.40 mA. Angiography is performed with a computed radiography system using iodine-based microspheres $15 \mu\text{m}$ in diameter. In angiography of nonliving animals, we observe fine blood vessels of approximately $100 \mu\text{m}$ with high contrasts. © 2005 Society of Photo-Optical Instrumentation Engineers. [DOI: 10.1117/1.2049268]

Subject terms: x-ray tube; cerium target; quasimonochromatic x-rays; characteristic x-rays; K-edge angiography.

Paper 040733R received Oct. 6, 2004; revised manuscript received Mar. 8, 2005; accepted for publication Mar. 11, 2005; published online Sep. 16, 2005. This paper is a revision of a paper presented at the SPIE conference on X-Ray Sources and Optics, August 2004, Denver, CO. The paper presented there appears (unrefereed) in SPIE Proceedings Vol. 5537.

1 Introduction

Monochromatic parallel x-ray beams are the basis of radiography using synchrotrons in conjunction with single crystals, and these beams have been employed to perform enhanced K-edge angiography¹⁻³ and x-ray phase imaging.⁴⁻⁶ In angiography, the beams with photon energies of approximately 35 keV are absorbed effectively by iodine-based contrast media. However, it is difficult to obtain sufficient machine times for various research projects, including medical applications. Subsequently, monochromatic cone beams with energies of approximately 35 keV are useful for increasing the irradiation field for K-edge angiography.

To perform high-speed medical radiography, although several different flash x-ray generators⁷⁻¹³ utilizing cold-cathode tubes have been developed, plasma flash x-ray generators¹⁴⁻¹⁸ are useful for producing quasimonochromatic x-rays without using a K-edge filter. Therefore, we have performed a demonstration of cone beam K-edge

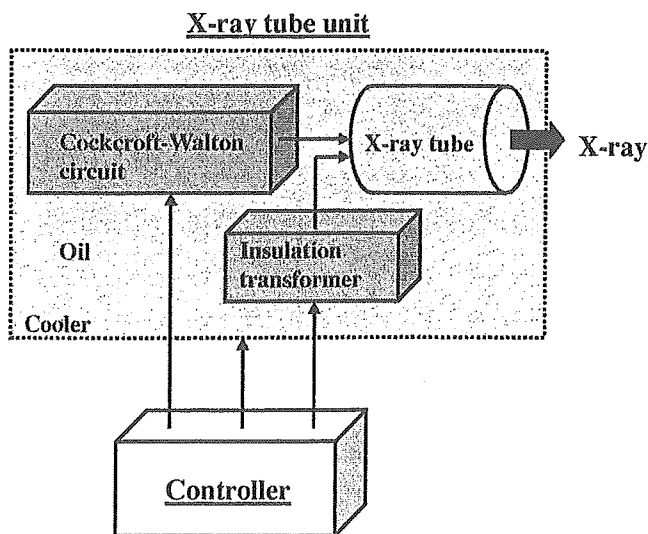


Fig. 1 Block diagram of the compact x-ray generator with a cerium-target radiation tube, which is used specially for K-edge angiography using iodine-based contrast media.

angiography¹⁹ utilizing a cerium plasma generator, since K-series characteristic x-rays from the cerium target are absorbed effectively by iodine.

Recently, we have developed a steady-state x-ray generator utilizing a cerium-target tube, and have demonstrated enhanced K-edge angiography utilizing cerium $K\alpha$ lines (34.6 keV).²⁰ In this research, $K\alpha$ lines were left by absorbing $K\beta$ lines (39.2 keV) using a barium sulfate filter with a barium K edge of 37.4 keV. However, because cerium $K\beta$ lines are also absorbed effectively by iodine, both $K\alpha$ and

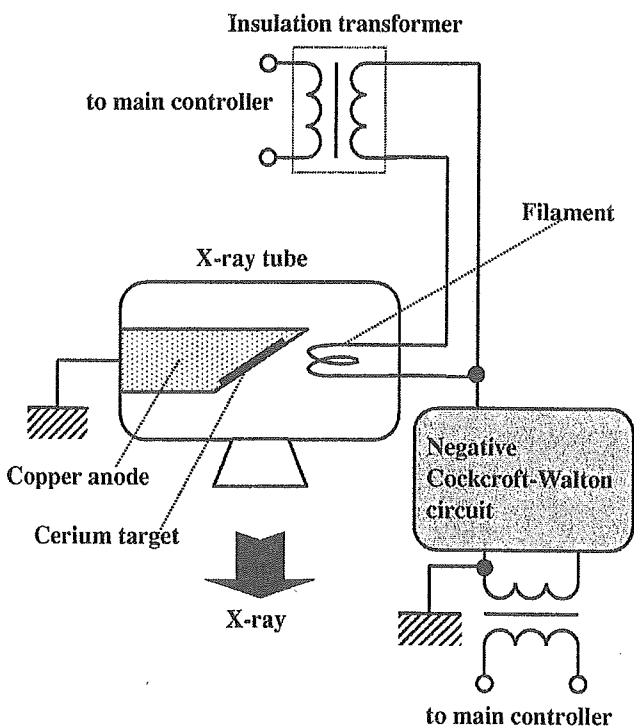


Fig. 2 Main circuit of the x-ray generator.

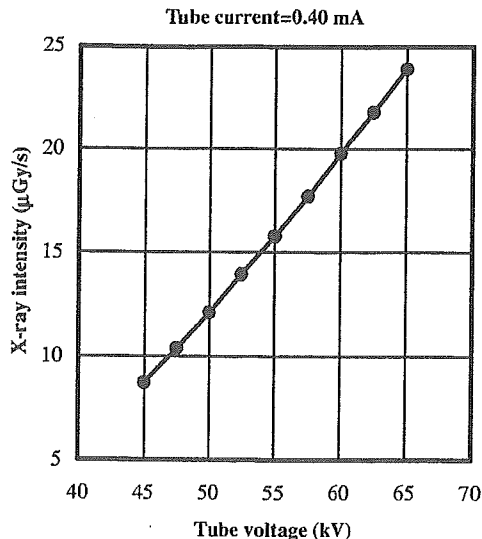


Fig. 3 The x-ray intensity ($\mu\text{Gy/s}$) as a function of tube voltage (kV) with a tube current of 0.40 mA.

$K\beta$ lines can be selected to increase the x-ray intensity for angiography. In measurements of x-ray spectra, although we usually employed a cadmium telluride detector with a photon energy resolution of 1.7 keV, the resolution should be minimized to measure the characteristic x-ray intensity.

In the present research, we measured the x-ray spectra from a cerium-target tube using a germanium detector, and performed a preliminary study on cone beam K-edge angiography achieved with cerium characteristic x-rays without using a K-edge filter.

2 Experimental Setup

Figure 1 shows the block diagram of the x-ray generator, which consists of a main controller and an x-ray tube unit with a Cockcroft-Walton circuit and a cerium-target tube. The tube voltage, the current, and the exposure time can be controlled by the controller. The main circuit for producing x-rays is illustrated in Fig. 2, and employs the Cockcroft-Walton circuit to decrease the dimensions of the tube unit. In the x-ray tube, the negative high voltage is applied to the cathode electrode, and the anode (target) is connected to the tube unit case (ground potential) to cool the anode and the target effectively. The filament heating current is supplied by an AC power supply in the controller in conjunction with an insulation transformer. In this experiment, the tube

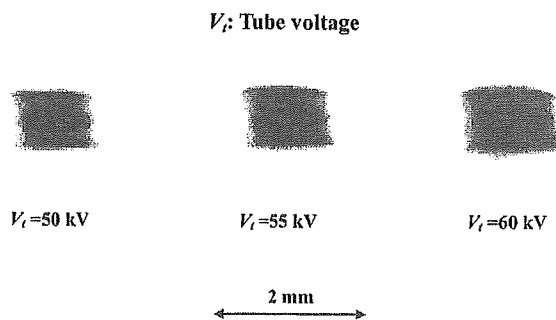


Fig. 4 Effective focal spots with changes in the tube voltage.

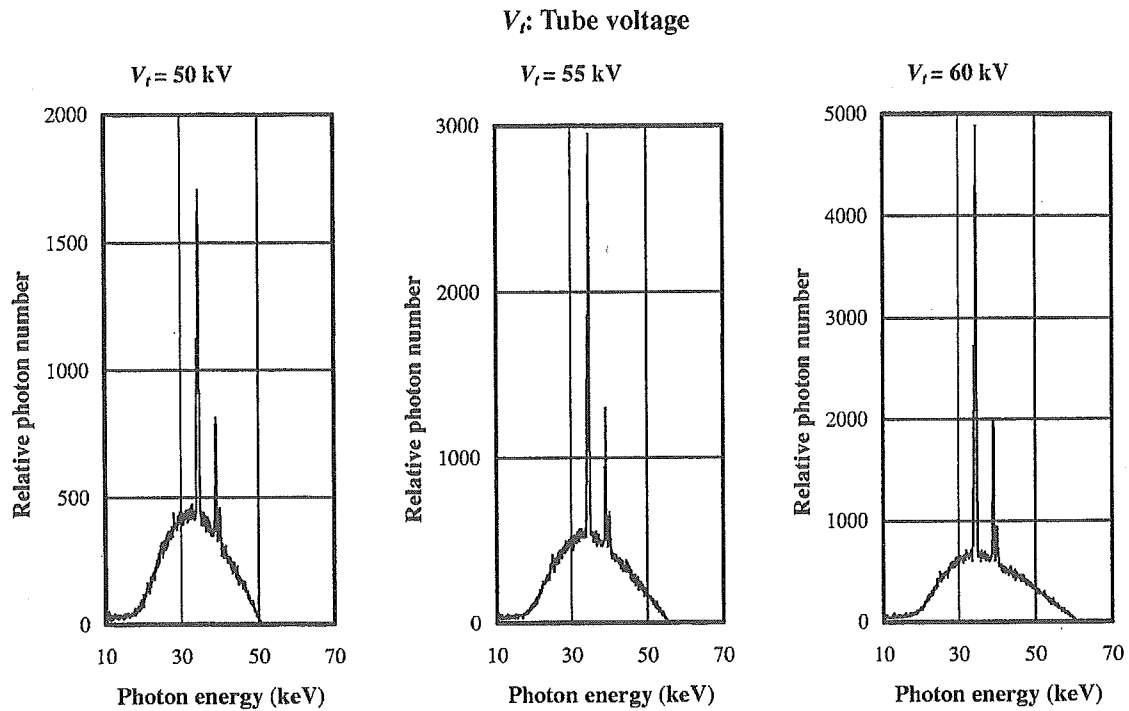


Fig. 5 X-ray spectra measured using a germanium detector with changes in the tube voltage.

voltage applied was from 45 to 65 kV, and the tube current was regulated to within 0.40 mA (maximum current) by the filament temperature. The exposure time is controlled to obtain optimum x-ray intensity. Quasimonochromatic x-rays are produced using a 3.0-mm-thick aluminum filter for absorbing soft bremsstrahlung rays.

3 Results and Discussion

3.1 X-ray Intensity

X-ray intensity was measured by a Victoreen 660 ionization chamber at 1.0 m from the x-ray source using the filter (Fig. 3). At a constant tube current of 0.40 mA, the x-ray intensity increased when the tube voltage was increased. In this measurement, the intensity with a tube voltage of 60 kV and a current of 0.40 mA was $19.9 \mu\text{Gy/s}$ at 1.0 m from the source, with errors of less than 0.2%.

3.2 Focal Spot

To measure images of the x-ray source after the aluminum filtration, we employed a pinhole camera with a hole diameter of $50 \mu\text{m}$ (magnification ratio of 1:2) in conjunction with a computed radiography (CR) system²¹ with a sampling pitch of $87.5 \mu\text{m}$. When the tube voltage was increased, spot dimensions increased slightly and had values of $1.3 \times 0.9 \text{ mm}$ (Fig. 4).

3.3 X-ray Spectra

To measure x-ray spectra, we employed a germanium detector (GLP-10180/07-P, Ortec Incorporated) with a photon energy resolution of approximately 0.12 keV (Fig. 5). When the tube voltage was increased, the characteristic x-ray intensities of $K\alpha$ and $K\beta$ lines substantially increased, and both the maximum photon energy and the intensities of bremsstrahlung x-rays increased. Because the widths of the lines were approximately 1 keV, the photon energy resolution of this detector was an optimum value. In an empirical equation, because the characteristic x-ray in-

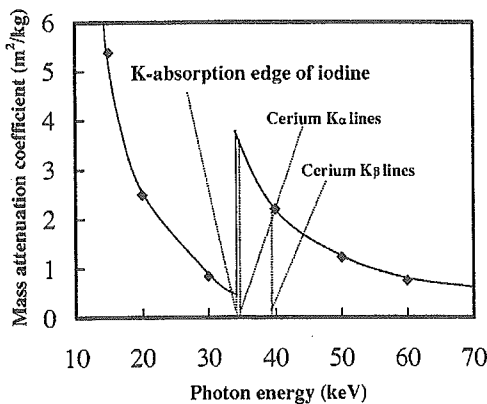


Fig. 6 Mass attenuation coefficients of iodine, and the average photon energies of cerium $K\alpha$ and $K\beta$ lines.

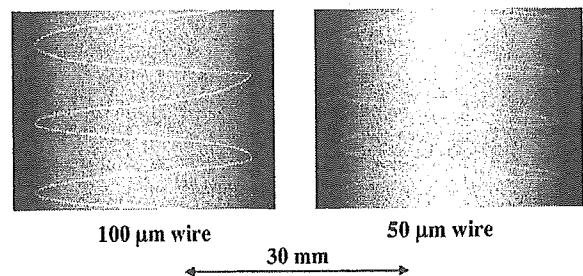


Fig. 7 Radiograms of tungsten wires coiled around PMMA rods with a tube voltage of 60 kV.

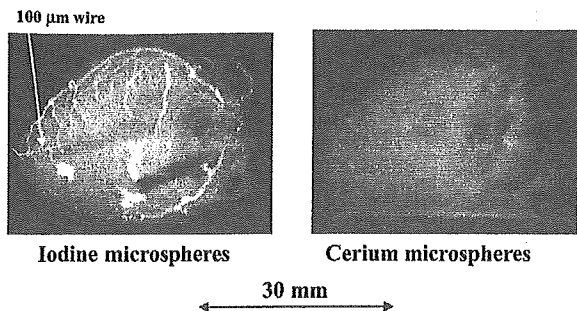


Fig. 8 Angiograms of extracted rabbit hearts using iodine and cerium microspheres with a tube voltage of 60 kV.

tensity is proportional to approximately 1.5 power of the voltage difference between the tube voltage and the critical excitation voltage, the measured intensities of the characteristic x-rays corresponded well to the equation.

3.4 K-Edge Angiography

Figure 6 shows the mass attenuation coefficients of iodine at the selected energies; the coefficient curve is discontinuous at the iodine K edge. The average photon energy of the cerium $K\alpha$ and $K\beta$ lines are shown just above the iodine K edge. The average photon energies of $K\alpha$ and $K\beta$ lines are 34.6 and 39.2 keV, respectively, and iodine contrast media with a K-absorption edge of 33.2 keV absorb the lines easily. Therefore, blood vessels were observed with high contrasts.

The angiography was performed by a CR system (Konica Minolta Regius 150) using the filter, and the distance (between the x-ray source and the imaging plate) was 1.5 m. First, rough measurements of spatial resolution were made using wires. Figure 7 shows radiograms of tungsten wires coiled around a rod made of polymethyl methacrylate. Although the image contrast decreased somewhat with decreases in the wire diameter, due to blurring of the image caused by the sampling pitch of $87.5 \mu\text{m}$, a $50\text{-}\mu\text{m}$ -diam wire could be observed.

Angiograms of rabbit hearts are shown in Fig. 8. These two images were obtained using iodine and cerium microspheres of $15 \mu\text{m}$ in diameter at a tube voltage of 60 kV.

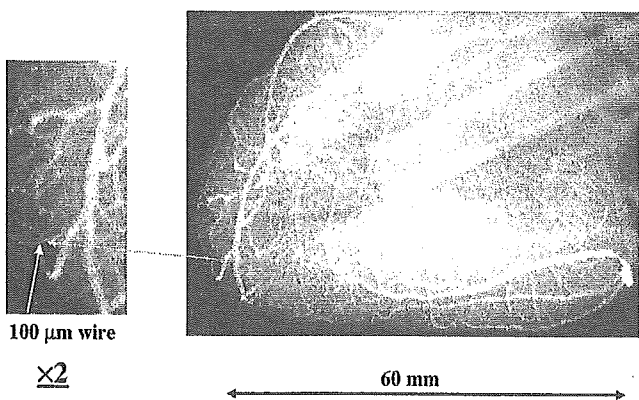


Fig. 9 Angiograms of an extracted dog heart using iodine microspheres with a tube voltage of 60 kV.

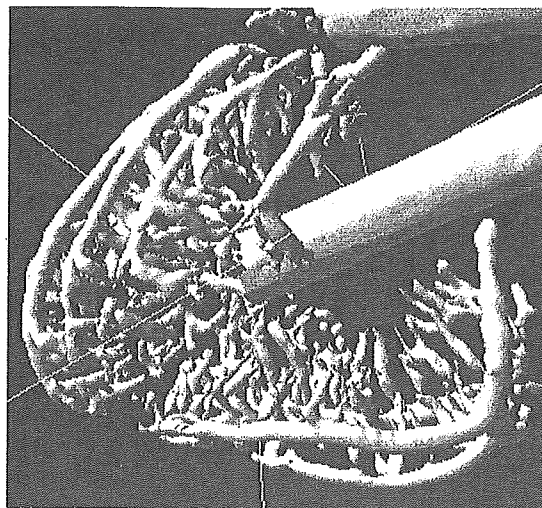


Fig. 10 3-D image of coronary arteries constructed from x-ray CT images by Pascal.

The microspheres are very useful for making phantoms of nonliving animals used for angiography. The iodine plastic spheres contained 37% iodine by weight, and the cerium plastic spheres were chemically stable and contained 18% cerium by weight. In the case where the cerium spheres were employed, the coronary arteries were barely visible, since the cerium spheres transmitted cerium characteristic x-rays easily. Figure 9 shows an angiogram of a larger dog heart at a tube voltage of 60 kV using iodine spheres. For comparison, we show a 3-D image of the coronary arteries constructed from x-ray CT images by Pascal (Digital Culture Technical Corporation) with a tungsten x-ray tube (Fig. 10). Using this imaging technique, fine blood vessels were not observed at all.

4 Conclusion and Outlook

In summary, we employ an x-ray generator with a cerium-target tube and succeed in producing cerium characteristic x-rays, which can be absorbed easily by iodine-based contrast media. The characteristic x-ray intensities increase with increases in the tube voltage, and low-photon-energy bremsstrahlung rays are absorbed effectively by the filter.

Although the cerium x-ray generator used in this research produces both the characteristic and the bremsstrahlung x-rays, bremsstrahlung intensity can be decreased effectively by considering the angle dependence without using the filter, since bremsstrahlung rays are not emitted in the opposite direction to that of electron trajectory in Sommerfeld's theory.²² Subsequently, the generator-produced maximum number of characteristic photons is approximately 3.5×10^7 photons/cm²·s at 1.0 m from the source, and the photon count rate can be increased easily by improving the target.

The x-ray intensity is limited because the thermal contact between the target and the anode is not good. However, the intensity can be increased by welding the target or using a cerium-alloy target. In addition, a rotation anode tube can be developed by the sputtering of cerium.

Compared to the 3-D blood images constructed from x-ray CT images by Pascal, fine blood vessels are visible.

Because the sampling pitch of the CR system is $87.5\ \mu\text{m}$, we obtain spatial resolutions of approximately $100\ \mu\text{m}$. To observe fine blood vessels of less than $100\ \mu\text{m}$, the spatial resolution of the CR system should be improved to approximately $50\ \mu\text{m}$ (Konica Minolta Regius 190). In addition, the spatial resolution can be improved easily to approximately $50\ \mu\text{m}$ or less in cases where an x-ray film (Fuji Ix 100) is employed.

Acknowledgment

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, and 16591222) and Advanced Medical Scientific Research from MECSST, Health and Labor Sciences Research Grants (RAMT-nano-001, RHGTEFB-genome-005, and RHGTEFB-saisei-003), grants from Keiryō Research Foundation, The Promotion and Mutual Aid Corporation for Private Schools of Japan, Japan Science and Technology Agency (JST), and New Energy and Industrial Technology Development Organization (NEDO, Industrial Technology Research Grant Program in 2003).

References

1. A. C. Thompson, H. D. Zeman, G. S. Brown, J. Morrison, P. Reiser, V. Padmanabhan, L. Ong, S. Green, J. Giacomini, H. Gordon, and E. Rubenstein, "First operation of the medical research facility at the NSLS for coronary angiography," *Rev. Sci. Instrum.* **63**, 625–628 (1992).
2. H. Mori, K. Hyodo, E. Tanaka, M. U. Mohammed, A. Yamakawa, Y. Shinozaki, H. Nakazawa, Y. Tanaka, T. Sekka, Y. Iwata, S. Honda, K. Umetani, H. Ueki, T. Yokoyama, K. Tanioka, M. Kubota, H. Hosaka, N. Ishizawa, and M. Ando, "Small-vessel radiography in situ with monochromatic synchrotron radiation," *Radiology* **201**, 173–177 (1996).
3. K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita, and J. Tada, "Development of a two-dimensional imaging system for clinical applications of intravenous coronary angiography using intense synchrotron radiation produced by a multipole wiggler," *J. Synchrotron Radiat.* **5**, 1123–1126 (1998).
4. T. J. Davis, D. Gao, T. E. Gureyev, A. W. Stevenson, and S. W. Wilkins, "Phase-contrast imaging of weakly absorbing materials using hard x-rays," *Nature (London)* **373**, 595–597 (1995).
5. A. Momose, T. Takeda, Y. Itai, and K. Hirano, "Phase-contrast x-ray computed tomography for observing biological soft tissues," *Nat. Med.* **2**, 473–475 (1996).
6. M. Ando, A. Maksimenko, H. Sugiyama, W. Pattanasiruwisawa, K. Hyodo, and C. Uyama, "A simple x-ray dark- and bright-field imaging using achromatic Laue optics," *Jpn. J. Appl. Phys., Part 2* **41**, L1016–L1018 (2002).
7. E. Sato, S. Kimura, S. Kawasaki, H. Isobe, K. Takahashi, Y. Tamakawa, and T. Yanagisawa, "Repetitive flash x-ray generator utilizing a simple diode with a new type of energy-selective function," *Rev. Sci. Instrum.* **61**, 2343–2348 (1990).
8. E. Sato, M. Sagae, K. Takahashi, T. Oizumi, H. Ojima, K. Takayama, Y. Tamakawa, T. Yanagisawa, A. Fujiwara, and K. Mitoya, "High-speed soft x-ray generators in biomedicine," *Proc. SPIE* **2513**, 649–667 (1994).
9. E. Sato, M. Sagae, K. Takahashi, A. Shikoda, T. Oizumi, H. Ojima, K. Takayama, Y. Tamakawa, T. Yanagisawa, A. Fujiwara, and K. Mitoya, "Dual energy flash x-ray generator," *Proc. SPIE* **2513**, 723–735 (1994).
10. A. Shikoda, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa, and T. Yanagisawa, "Repetitive flash x-ray generator having a high-durability diode driven by a two-cable-type line pulser," *Rev. Sci. Instrum.* **65**, 850–856 (1994).
11. E. Sato, K. Takahashi, M. Sagae, S. Kimura, T. Oizumi, Y. Hayasi, Y. Tamakawa, and T. Yanagisawa, "Sub-kilohertz flash x-ray generator utilizing a glass-enclosed cold-cathode triode," *Med. Biol. Eng. Comput.* **32**, 289–294 (1994).
12. K. Takahashi, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa, and T. Yanagisawa, "Fundamental study on a long-duration flash x-ray generator with a surface-discharge triode," *Jpn. J. Appl. Phys., Part 1* **33**, 4146–4151 (1994).
13. E. Sato, M. Sagae, A. Shikoda, K. Takahashi, T. Oizumi, M. Yamamoto, A. Takabe, K. Sakamaki, Y. Hayasi, H. Ojima, K. Takayama, and Y. Tamakawa, "High-speed soft x-ray techniques," *Proc. SPIE* **2869**, 937–955 (1996).
14. E. Sato, Y. Hayasi, E. Tanaka, H. Mori, T. Kawai, T. Usuki, K. Sato, H. Obara, T. Ichimaru, K. Takayama, H. Ido, and Y. Tamakawa, "Quasi-monochromatic radiography using a high-intensity quasi-x-ray laser generator," *Proc. SPIE* **4682**, 538–548 (2002).
15. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, H. Obara, T. Ichimaru, K. Takayama, and H. Ido, "Intense characteristic x-ray irradiation from weakly ionized linear plasma and applications," *Jpn. J. Med. Imag. Inform. Sci.* **20**, 148–155 (2003).
16. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, H. Obara, T. Ichimaru, K. Takayama, and H. Ido, "Irradiation of intense characteristic x-rays from weakly ionized linear molybdenum plasma," *Jpn. J. Med. Phys.* **23**, 123–131 (2003).
17. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama, and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing weakly ionized linear copper plasma," *Rev. Sci. Instrum.* **74**, 5236–5240 (2003).
18. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama, and H. Ido, "Sharp characteristic x-ray irradiation from weakly ionized linear plasma," *J. Electron Spectrosc. Relat. Phenom.* **137–140**, 713–720 (2004).
19. E. Sato, R. Germer, Y. Hayasi, K. Murakami, Y. Koorikawa, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, F. Obata, K. Takahashi, S. Sato, K. Takayama, and H. Ido, "Weakly ionized cerium plasma radiography," *Proc. SPIE* **5210**, 12–21 (2003).
20. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama, and H. Ido, "Demonstration of enhanced K-edge angiography using a cerium target x-ray generator," *Med. Phys.* **31**, 3017 (2004).
21. E. Sato, K. Sato, and Y. Tamakawa, "Film-less computed radiography system for high-speed imaging," *Ann. Rep. Iwate Med. Univ. Sch. Lib. Arts Sci.* **35**, 13–23 (2000).
22. B. K. Agarwal, *X-Ray Spectroscopy*, 2nd ed., p. 18, Springer-Verlag, New York (1991).

Eiichi Sato received his BS, MS, and PhD in applied physics from Tohoku Gakuin University, Sendai, Japan, in 1979, 1982, and 1987, respectively. He is currently a professor in the Department of Physics at Iwate Medical University. He has written approximately 400 publications and delivered 200 international presentations concerning x-rays. His research interests include soft flash x-ray generators, quasi-x-ray laser generators, and high-speed radiography. In 2000, he received the Schardin Gold Medal from the German Physical Society, in 2003 he received the Takayama Award (Gold Medal) from the Japan Society of High Speed Photography and Photonics, and he received the Honorable Mention Poster Award from the SPIE International Symposium on Medical Imaging 2005.

Akira Yamadera received his BS, MS, and PhD degrees in physics from Tohoku University in 1969, 1971, and 1978, respectively. He is currently a professor in the Department of Radiological Technology, School of Health Sciences at Hirosaki University. His research interests include radiation dose measurement using imaging plates, radiation safety, environmental radiation measurements, and x-ray spectroscopy.

Etsuro Tanaka received his MD and PhD degrees in medicine from Kumamoto University, Japan, in 1980 and 1986, respectively. He worked on medical image processing in the Department of Physiology, Tokai University, Japan, from 1988 to 2003. He is currently a professor in the Department of Nutritional Sciences, Tokyo University of Agriculture, Japan. His research interests include medical image processing, human physiology, and clinical nutrition.

Hidezo Mori received a medical degree from Keio University School of Medicine, Tokyo, Japan, in 1977, and also a PhD from the Post Graduate School, Keio University School of Medicine. Now he is the director of the Department of Cardiac Physiology at the National Cardiovascular Center, Suita, Japan. His primary research interests are regenerative therapy in cardiovascular disease, microcirculation, and medical applications of structural biology.

Toshiaki Kawai received the BS degree in precision mechanics and the MS degree in electronic engineering from Shizuoka University, Hamamatsu, Japan, in 1964 and 1974, respectively. In 1974, he joined the Hamamatsu Photonics K.K., where he worked on research and development of solid-state infrared detectors, and then from 1978 to 1981 engaged in research work on the NEA cold cathode for application to imaging camera tubes. He is now the project coordinator of Electron Tube Division 2 and is engaged in the development and manufacturing of imaging devices and x-ray equipment. He is a member of the Japan Radioisotope Association and the Institute of Image Information and Television Engineers of Japan.

Fumihito Ito left the Department of Mechanical Engineering, Iwate University, in 2001. Since 2002, he has been a member of the research and development section of the Digital Culture Technology Corporation, Japan. Since 2004 he has been a student on the doctoral course in the Faculty of Software and Information Science at Iwate Prefectural University. His research interests include 3-D imaging reconstructed from images in optical coherence tomography (OCT), x-ray CT, and MRI.

Takashi Inoue received his MD and PhD degrees in 2000 from Tohoku University. He is currently an assistant professor in the Department of Neurosurgery at Iwate Medical University, and a member of the Japan Neurosurgical Society. His research interests include neurosurgery and MRI.

Akira Ogawa received his MD and PhD degrees in 1981 from Tohoku University. He is currently a professor in the Department of Neurosurgery and Dean of the School of Medicine at Iwate Medical University, and is a trustee of the Japan Neurosurgical Society. His research interests include neurosurgery and cerebrovascular disease.

Shigehiro Sato received his MD degree from Iwate Medical University in 1980. He worked for the laboratory of the Division of Pediatric Infectious Diseases at Johns Hopkins Hospital from 1985 to 1989. He is currently a professor in the Department of Microbiology at Iwate Medical University. His research interests include central nervous system damage caused by Vero toxin, a cell culture system for vaccine development, and microangiography.

Kazuyoshi Takayama received his BS degree from Nagoya Institute of Technology in 1962. In 1970, he received his PhD in mechanical engineering from Tohoku University. He is currently a director (professor) in the Shock Wave Research Center, Institute of Fluid Science at Tohoku University. His research interests include various shock wave phenomena, high speed photography, and flash radiography. He has received seven awards, including the coveted Ernst Mach Medal in 2000.

Jun Onagawa received his BS and PhD degrees in physics from Tohoku Gakuin University in 1968 and 2001, respectively. He is currently a professor in the Department of Applied Physics and Informatics, Faculty of Engineering, at Tohoku Gakuin University. His research interests include target metallography and x-ray spectroscopy.

Hideaki Ido received his BS, MS, and PhD degrees in physics from Tohoku University in 1962, 1964, and 1967, respectively. He is currently a professor in the Department of Applied Physics and Informatics, Faculty of Engineering, at Tohoku Gakuin University. His research interests include magnetism and x-ray spectroscopy.

EXOGENOUS NITRIC OXIDE CENTRALLY ENHANCES PULMONARY REACTIVITY IN THE NORMAL AND HYPERTENSIVE RAT

Daryl O Schwenke,* James T Pearson,* Hirotsugu Tsuchimochi,* Hidezo Mori* and Mikiyasu Shirai†

*Department of Cardiac Physiology, National Cardiovascular Center Research Institute, Suita, Osaka and

†Faculty of Health Sciences, Hiroshima International University, Hiroshima, Japan

SUMMARY

1. Chronic hypoxia causes sustained pulmonary hypertension and, although impairment of the pulmonary endothelial nitric oxide (NO) pathway has been implicated, no study has described the central role of NO in modulating pulmonary vascular tone and reactivity. Centrally, NO inhibits sympathetic outflow, so we hypothesised that central NO would modulate pulmonary vascular tone and its reactivity to acute hypoxia, especially in the hypertensive state.

2. Male adult Sprague-Dawley rats were exposed to normoxia (N) or chronic hypoxia (CH; 12% O₂) for 14 days. Mean pulmonary arterial pressure (MPAP), systemic mean arterial blood pressure (MABP), cardiac output and heart rate were then measured in pentobarbitone-anaesthetized, artificially ventilated rats. The N and CH rats were exposed to acute hypoxia (10% O₂ for 4 min) after the intracerebroventricular (i.c.v.) administration of artificial cerebrospinal fluid (control) and then again after either i.c.v. N^G-nitro-L-arginine methyl ester (L-NAME; 150 µg in 10 µL) or 3-morpholino-sydnonimine hydrochloride (SIN-1; 100 µg in 10 µL).

3. Chronic hypoxia caused pulmonary hypertension (MPAP 20 ± 1 vs 30 ± 1 mmHg in N and CH rats, respectively) and attenuated acute hypoxic pulmonary vasoconstriction (HPV). Central inhibition of NO synthesis (by L-NAME) did not alter baseline MPAP or the acute HPV in either N or CH rats, but it did elevate MABP. The NO donor SIN-1 did not alter baseline MPAP, but it did enhance (N rats) or restore (CH rats) the HPV and decreased MABP.

4. The results of the present study indicate that central NO has a limited role in the tonic modulation of MPAP during normoxia and after chronic hypoxia. However, the acute HPV seems to be enhanced by exogenous NO.

Key words: chronic hypoxia, nitric oxide, pulmonary vasoconstriction, sympathetic nervous system.

INTRODUCTION

Acute alveolar hypoxia causes pulmonary vasoconstriction that is reversible upon re-oxygenation. However, during chronic hypoxia, as is the case with several chronic pulmonary pathological conditions, elevated shear stress within the pulmonary vasculature causes endothelial cell injury/dysfunction,¹ smooth muscle cell proliferation² and, inevitably, the irreversible remodelling of the pulmonary vasculature.^{3,4} The consequential sustained increase in pulmonary arterial pressure (PAP) increases the workload of the heart and is therefore closely associated with heart failure and increased mortality.

Although the exact cellular mechanisms responsible for the pathogenesis of chronic hypoxia-induced pulmonary arterial hypertension are unknown, alterations in the endothelial nitric oxide (NO) pathway have been implicated as a significant contributing factor.^{5,6} Nitric oxide is a potent vasodilator and an inhibitor of vascular remodelling.^{7–9} Nitric oxide is produced from L-arginine in a reaction catalysed by isoenzymes of NO synthase (NOS). The synthesis of NO is blocked by several L-arginine analogues, including N^G-nitro-L-arginine methyl ester (L-NAME), which competitively and stereoselectively inhibit the generation of NO from L-arginine.¹⁰

A reduction in the production of NO has been implicated in the pathophysiology of pulmonary hypertension.^{6,8} Endothelial NOS (eNOS)-knockout mice have an increased risk of pulmonary hypertension,^{11–13} whereas the hypoxia-induced pulmonary hypertension is attenuated in transgenic mice that overexpress eNOS.¹⁴ In addition, chronic hypoxia limits endogenous NO synthesis,¹⁵ despite an increase in NOS expression.^{16–18}

Nitric oxide is produced not only peripherally, but also centrally within various parts of the brain, including the nucleus tractus solitarius (NTS) of the medulla oblongata and the ventrolateral medulla, the cardiovascular regulatory centres.^{19–21} Therefore, NO is considered to be involved in the neural regulation of blood pressure, independent of its direct effects on the endothelium of blood vessels.²² A review by Patel *et al.*²³ reported that the general consensus in the literature was that NO acts as a sympatho-inhibitory substance within the central nervous system. Therefore, central NO inhibition increases sympathetic outflow and, subsequently, arterial blood pressure.^{24,25}

The central role of NO in modulating pulmonary vasculature, especially in pathological conditions (e.g. pulmonary hypertension), is still incompletely understood. Yet, as evidence accumulates in support of central NO as an important regulator

Correspondence: Daryl O Schwenke, Department of Cardiac Physiology, National Cardiovascular Center Research Institute, 5-7-1 Fujishirodai, Suita, Osaka 565-8565, Japan. Email: schwenke@ri.ncvc.go.jp

Received 2 March 2005; revision 1 June 2005; accepted 17 July 2005.

© 2005 Blackwell Publishing Asia Pty Ltd

of cardiovascular function, the central role of NO in the modulation of the pulmonary vasculature needs to be addressed. Therefore, our first aim in the present study was to elucidate the role of NO in the central modulation of pulmonary vascular tone under normoxic conditions and after the development of chronic hypoxia-induced pulmonary hypertension. Nitric oxide is thought to have an important role in modulating the hypoxic pulmonary vasoconstriction (HPV) in response to acute hypoxic challenges.²⁶ However, there are conflicting reports as to whether the HPV response is accentuated or attenuated by pulmonary hypertension.^{6,27} Therefore, a second aim of the present study was to assess the acute HPV before and after chronic hypoxia and to determine whether central NO has a role in modulating this response.

METHODS

Animals

Experiments were conducted on 23 male Sprague-Dawley rats (8 weeks old; bodyweight approximately 200–280 g). Rats were divided into four groups, as follows: (i) group 1, normoxia (N) + L-NAME; (ii) group 2, chronic hypoxia (CH) + L-NAME; (iii) group 3, N + 3-morpholino-sydnimine hydrochloride (SIN-1); and (iv) group 4, CH + SIN-1. The CH rats were housed in a hypoxic chamber ($12.0 \pm 0.1\%$ O₂) continuously for 2 weeks, except for a 10 min interval each day when the chamber was cleaned. The N rats were housed in similar housing, except that N rats breathed room air. The hypoxic gas mixture was delivered to the hypoxic chamber (30 L capacity) at a flow rate of approximately 8 L/min. All rats were on a 12 h light/dark cycle at $25 \pm 1^\circ\text{C}$ and were provided with food and water *ad libitum*. All experiments were approved by the local Animal Ethics Committee and conducted in accordance with the guidelines of the Physiological Society of Japan (<http://www.soc.nii.ac.jp/psj/>).

Anaesthesia and surgery

Rats were initially anaesthetized with pentobarbitone sodium (45 mg/kg, i.p.) and supplementary doses of anaesthetic were administered periodically throughout the experimental protocol (15–30 mg/kg per h, i.p.) so as to maintain a constant surgical level of anaesthesia (assessed by using the limb withdrawal reflex test). Rectal temperature was maintained at 38°C using a rectal thermistor coupled to a thermostatically controlled heating pad.

Using a stereotaxic frame, the tip of a 27 gauge stainless steel cannula was positioned in the right lateral cerebral ventricle based on the coordinates of Paxinos and Watson²⁸ (0.8 mm posterior to the bregma, 1.5 mm lateral to the midline and 5.0 mm ventral to the skull surface). The distal end of the cannula was connected to a 0.5 mL syringe for subsequent drug administration. Correct positioning of the intracerebroventricular (i.c.v.) catheter was confirmed after each experiment by staining with Evans blue dye (10 μL).

The trachea was cannulated and the lungs ventilated with a rodent ventilator (SN-480-7; Shinano, Tokyo, Japan). The inspirate gas was enriched with O₂ (approximately 50% O₂) and the ventilator settings were adjusted (tidal volume (V_T) approximately 3.5 mL; frequency approximately 80 /min) to maintain arterial P_{CO2} normocapnic. The femoral artery and vein were cannulated for the measurement of systemic arterial blood pressure and drug administration, respectively. The arterial line contained heparinized saline (50 U/mL). A right thoracotomy was made between the second and third ribs and the conus of the right ventricle was exposed. A 23 gauge needle was used to pierce the ventricle wall and then the gel-filled sensing catheter of a telemetric transmitter (model TA11PA-C40; Data Sciences, St Paul, MN, USA) was inserted anteriorly into the right ventricle and advanced into the pulmonary artery. The catheter was fixed in position with a 7.0 Prolene suture to the pericardium. The aorta was bluntly dissected free from the pulmonary artery and a transonic perivascular flowprobe

(model 2RB; Transonic Systems, Ithaca, NY, USA) was positioned around the ascending aorta for the continuous measurement of cardiac output.

Drugs

Artificial cerebrospinal fluid (aCSF) was used as the vehicle for administering the NOS inhibitor L-NAME and the slow-releasing NO donor, 3-[4-morpholinyl]-sydnimine-hydrochloride (SIN-1). The aCSF (pH 7.36–7.43) was comprised of 150 mmol/L NaCl, 3.0 mmol/L KCl, 0.8 mmol/L MgCl₂, 1.4 mmol/L CaCl₂ and 1.0 mmol/L Na phosphate. Intracerebroventricular injections were given as a 10 μL bolus over 30 s. Intravenous (i.v.) injections were administered as a 0.2 mL bolus over 15 s, followed by a 0.1 mL saline flush.

Measurement of right ventricular weight

Immediately following the experiment, rats were killed by anaesthetic overdose, the heart was excised, the atria were removed and the right ventricle wall was separated from the left ventricle, including the septum. Tissues were blotted and weighed. Right and left ventricular weights were expressed as the ratio of the right ventricle to the left ventricular + septum weight ($W_{RV}/W_{LV+septum}$; Fulton's ratio).

Experimental protocols

Once all variables had stabilized after surgery (approximately 20 min), baseline values were recorded for 10 min in response to the i.c.v. administration of aCSF (10 μL). The inspirate was then switched to hypoxia (10% O₂ balanced by N₂) for 4 min. Upon recovery from acute hypoxia, rats received a bolus i.c.v. injection of either L-NAME (150 μg ; groups 1 and 2) or SIN-1 (100 μg ; groups 3 and 4). After 5 (L-NAME) or 10 min (SIN-1), the acute hypoxic test was repeated. After a further 10 min, once variables had recovered to prehypoxic values, rats (groups 1 and 2 only) received a bolus i.v. injection of L-NAME (50 mg/kg) and acute hypoxia was tested 10 min later.

Data acquisition and analysis

Pulmonary arterial pressure was measured using telemetry. The signal from the implanted transmitter (model TA11PA-C20; Data Sciences) was calibrated in reference to an input from an ambient-pressure monitor (C11PR; Data Sciences) and subsequently relayed to a personal computer. Cardiac output (CO) was measured continuously from the ascending aorta using a Transonic small animal blood flowmeter (model T206; Transonic Systems) with a flowprobe (model 2RB). Arterial blood pressure (ABP) was measured continuously with a Deltran pressure transducer (Utah Medical Products, Midvale, UT, USA) and the signal was relayed to a Powerlab bridge amplifier (ML117; ADInstruments, Tokyo, Japan).

The signals for ABP, CO and PAP were relayed from their respective units and sampled continuously at 200 Hz with an eight-channel MacLab/8s interface hardware system (ADInstruments) and recorded on a Macintosh Power Book G4 using Chart (v. 5.0.1; ADInstruments). Heart rate (HR) was derived from the arterial systolic peaks. Cardiac output was normalized (off-line) to 100 g bodyweight. Total systemic vascular resistance (SVR) and total pulmonary vascular resistance (PVR) were calculated by dividing mean ABP (MABP) and mean PAP (MPAP) by the normalized CO. A 10 block of data was analysed –60, –30 s and immediately before (time '0') acute hypoxic exposure and then after 20, 40, 60, 90, 120, 180 and 240 s of exposure to 10% O₂. Normoxic data for individual rats in each group were averaged from values acquired at –60, –30 s and at time 0. An arterial blood sample (0.1 mL) was extracted 5 min after the completion of surgery for analysis of arterial P_{CO2} using an ABL 605 blood gas analyser (Radiometer, Copenhagen, Denmark). An additional 0.1 mL was extracted to measure haematocrit.

Statistical analysis

All statistical analyses were conducted using Statview (v. 5.01; SAS Institute, Cary, NC, USA). All results are presented as the mean \pm SEM. Two-way ANOVA (repeated measures) was used to test significance for: (i) changes in each variable in response to 4 min of acute hypoxia; and (ii) whether the hypoxic response was altered by drug administration (i.c.v. or i.v.).

One-way ANOVA (factorial) was used to test for differences in baseline values for normoxic and chronic hypoxic groups of rats. Where statistical significance was reached, post hoc analyses were incorporated using the paired or unpaired *t*-test with Dunnett's correction for multiple comparisons. $P \leq 0.05$ was predetermined as the level of significance for all statistical analyses.

RESULTS

Chronic hypoxia induced pulmonary hypertension (Table 1), as evidenced by the observation that the MPAP and PVR of CH rats ($n = 11$) was 50 and 34% higher, respectively, than that of normoxic (N) rats ($n = 12$; $P < 0.01$). Consequently, CH rats developed right ventricular hypertrophy (Δ RV/LV + Sep ratio of 0.23). Chronic hypoxia did not significantly change MABP or CO, but it did cause a significant reduction in HR (Δ HR 37 b.p.m.; $P < 0.01$), suggesting that the development of right ventricular hypertrophy resulted in an increase in stroke volume. An increase in haematocrit (Δ Hct 18%; $P < 0.001$) also occurred in CH.

Responses to acute hypoxia

In N rats, acute exposure to 10% O₂ provoked an increase in MPAP, after a latency of 65–88 s, which reached a plateau after approxi-

mately 180 s (Fig. 1a). By 4 min, MPAP had increased significantly by $31 \pm 5\%$, in spite of a small, albeit not significant, decline in both HR ($6 \pm 1\%$) and CO ($16 \pm 6\%$), reflecting substantial pulmonary vasoconstriction ($67 \pm 13\%$ increase in PVR). Acute hypoxia also provoked a $56 \pm 2\%$ decrease in MABP by the end of the 4th min, which was primarily due to systemic vasodilatation ($46 \pm 3\%$ decrease in SVR; Fig. 1a). Although CH slightly altered baseline values (detailed above), the magnitude of the response to 4 min hypoxia for MABP, HR, CO and SVR was essentially the same for the CH and N groups of rats (Fig. 1a,b). However, the potent pulmonary vasoconstriction seen in N rats was abolished in CH rats. Consequently, exposure to 10% O₂ did not cause a significant increase in MPAP or PVR in CH rats.

Administration of L-NAME

The maximum cardiovascular responses following a single i.c.v. injection of L-NAME are given in Table 2. In N rats, L-NAME caused a small (<3% increase) but consistent increase in PVR ($P < 0.05$), although MPAP was not significantly affected. In addition, L-NAME caused a maximal $15 \pm 4\%$ increase in MABP after 35 ± 8 s, which was solely attributed to systemic vasoconstriction ($16 \pm 4\%$ increase in SVR). All other variables were unaltered. The PVR, MABP and SVR responses were brief, returning to pre-L-NAME values within 4.5 min. Consequently, because acute hypoxia was tested 5 min after L-NAME injection, the prehypoxia baseline data were similar before and after L-NAME treatment. Furthermore, the magnitude of the cardiovascular responses to L-NAME for CH rats was statistically similar to that of N rats (Table 2). The i.c.v. administration of L-NAME did

Table 1 Baseline cardiovascular variables in rats exposed to normoxic or chronic hypoxia

	N rats	CH rats
MPAP (mmHg)	20.2 \pm 1.1	30.4 \pm 1.2**
MABP (mmHg)	106 \pm 6	118 \pm 4
CO (mL/min/100 g)	11.17 \pm 0.75	12.32 \pm 0.53
HR (b.p.m.)	416 \pm 8	379 \pm 11*
SVR (mmHg/mL per min per 100 g)	9.73 \pm 0.64	9.72 \pm 0.53
PVR (mmHg/mL per min per 100 g)	1.88 \pm 0.14	2.52 \pm 0.15*
RV/LV + Septum	0.31 \pm 0.01	0.55 \pm 0.02**
Haematocrit (%)	47 \pm 1	65 \pm 1**

Data are the mean \pm SEM. * $P < 0.01$, ** $P < 0.001$ compared with normoxia values.

N, normoxic rats (groups 1 and 3; $n = 12$); CH, chronic-hypoxic rats (12% O₂ for 2 weeks; groups 2 and 4; $n = 11$); MPAP, mean pulmonary arterial pressure; MABP, mean arterial blood pressure; CO, cardiac output; HR, heart rate; SVR, systemic vascular resistance; PVR, pulmonary vascular resistance; RV, right ventricle; LV, left ventricle.

Table 2 Maximum responses to intracerebroventricular N^G-nitro-L-arginine methyl ester (150 μ g in 10 μ L) in normoxic rats ($n = 7$) and chronic hypoxic rats ($n = 5$)

	Pre-L-NAME	Normoxia Max L-NAME	Pre-L-NAME	Chronic hypoxia Max L-NAME
MPAP (mmHg)	18.6 \pm 0.6	19.0 \pm 0.6	30.4 \pm 1.6	31.1 \pm 1.9
MABP (mmHg)	102 \pm 10	116 \pm 8**	110 \pm 5	120 \pm 5*
CO (mL/min per 100 g)	10.12 \pm 1.10	10.09 \pm 1.13	12.24 \pm 1.07	11.98 \pm 1.00
HR (b.p.m.)	413 \pm 10	416 \pm 9	373 \pm 13	376 \pm 14
SVR (mmHg/mL per min per 100 g)	10.79 \pm 1.85	12.39 \pm 2.05**	9.14 \pm 0.55	10.19 \pm 0.66*
PVR (mmHg/mL per min per 100 g)	1.94 \pm 0.20	2.00 \pm 0.21*	2.53 \pm 0.18	2.64 \pm 0.21*

Data are the mean \pm SEM. * $P < 0.05$, ** $P < 0.01$ compared with pre-N^G-nitro-L-arginine methyl ester (L-NAME).

MPAP, mean pulmonary arterial pressure; MABP, mean arterial blood pressure; CO, cardiac output; HR, heart rate; SVR, systemic vascular resistance; PVR, pulmonary vascular resistance.

not alter the acute hypoxic response for any of the variables recorded in either N or CH rats (Fig. 1a,b).

Cardiovascular responses to the i.v. administration of L-NAME (50 mg/kg, i.v.) were also recorded. In N rats, a bolus i.v. dose of L-NAME provoked robust systemic vasoconstriction ($123 \pm 20\%$ increase in SVR; $P < 0.001$), as well as, to a lesser extent, pulmonary vasoconstriction ($80 \pm 10\%$ increase in PVR; $P < 0.01$). The baroreflex decrease in HR and CO (NS; see baseline data in Fig. 1a,b) meant that the changes in vascular resistance were accompanied by smaller, but still significant, increases in MABP ($42 \pm 18\%$ increase in MABP; $P < 0.001$) and MPAP ($13 \pm 9\%$ increase in MPAP; NS) in N rats. After 2 weeks of chronic hypoxia, L-NAME (i.v.) had a similar effect on the systemic vasculature and caused a similar depression of HR (NS) and CO ($P < 0.001$), but it had a more pronounced effect on the pulmonary vasculature ($24 \pm 5\%$ increase in MPAP (NS); $116 \pm 18\%$ increase in PVR ($P < 0.01$)).

Treatment of N rats with L-NAME (i.v.) exacerbated the reduction in MABP and SVR in response to acute hypoxia and accentuated the increase in MPAP and PVR (Fig. 1a,b). Despite a depression in baseline values for CO and HR, i.v. administration of L-NAME did not change the transient responses to hypoxia. In CH rats, the transient MABP and SVR responses to acute hypoxia were elevated by L-NAME (i.v.). In addition, L-NAME restored the potent MPAP (and PVR) response to acute hypoxia (observed in N rats), which had been absent prior to L-NAME treatment (Fig. 1a,b).

Administration of SIN-1

Following a single bolus i.c.v. injection of SIN-1 (100 μg) in N rats, baseline MPAP and PVR were not significantly altered. However, MABP declined slowly before stabilizing $38 \pm 7\%$ below the pre-SIN-1 baseline (Table 3). Preliminary studies

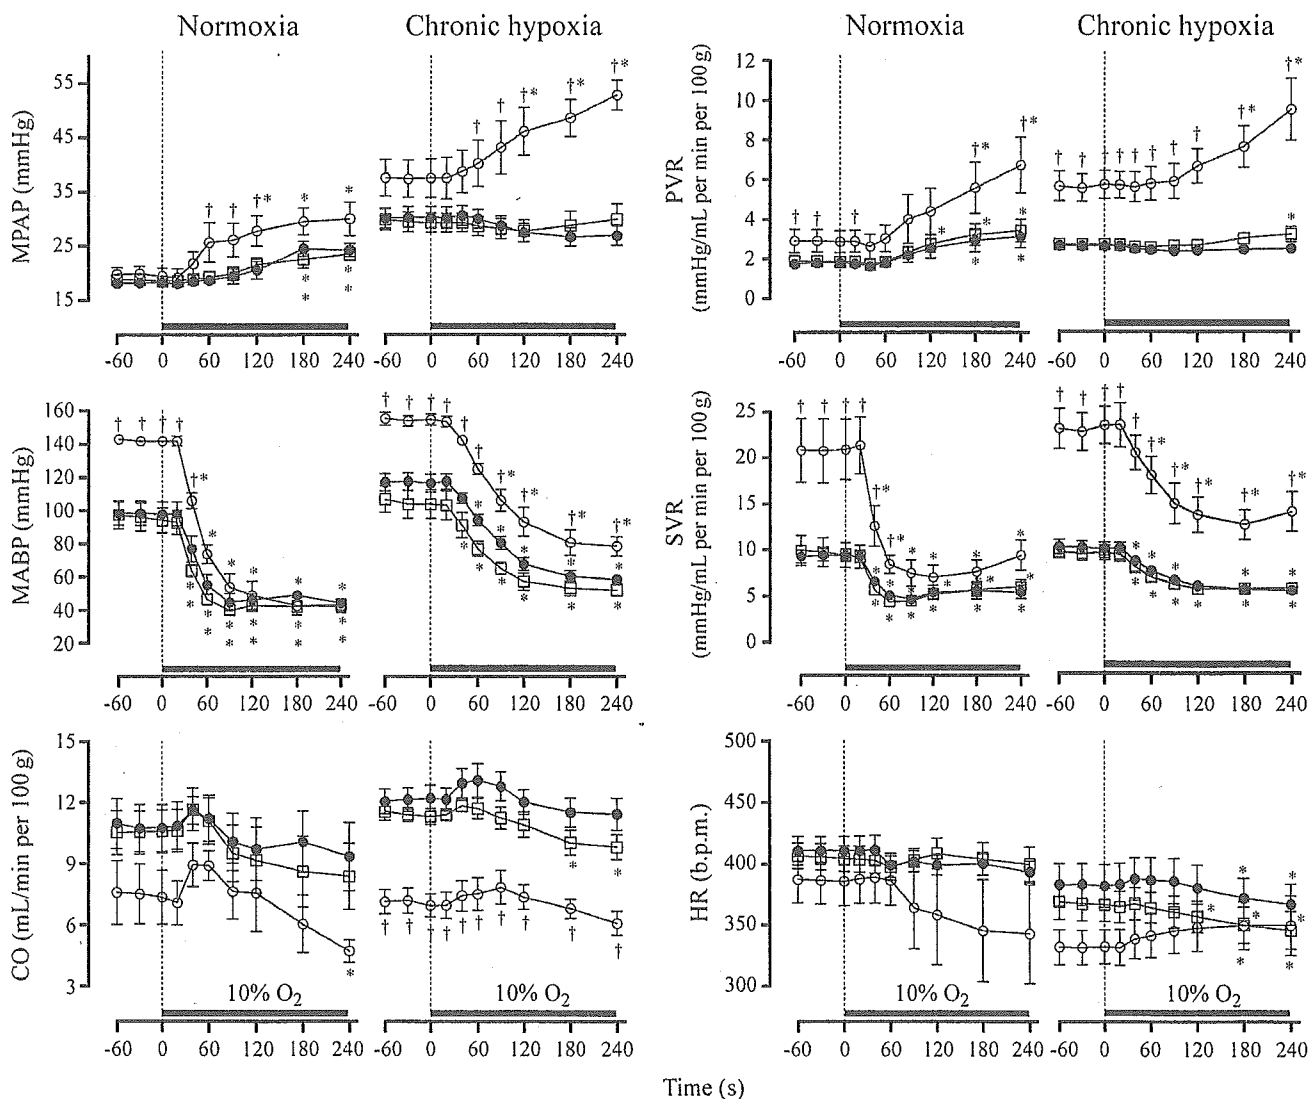


Fig. 1 Mean pulmonary arterial pressure (MPAP), mean arterial blood pressure (MABP), cardiac output (CO), pulmonary vascular resistance (PVR), systemic vascular resistance (SVR) and heart rate (HR) responses to acute hypoxia (10% O₂ for 4 min) in normoxic (N) rats ($n = 7$) and chronic hypoxic (CH) rats ($n = 5$), before (●) and after the administration of N^G-nitro-L-arginine methyl ester (L-NAME; □, 150 μg in 10 μL , i.c.v.; ◇, 50 mg/kg, i.v.). * $P < 0.05$ compared with pre-acute hypoxia values; † $P < 0.05$ compared with L-NAME values.

showed that once cardiovascular variables stabilized following the initial response to SIN-1, variables did not change for at least another 20 min. The fall in MABP was primarily attributed to vasodilatation ($29 \pm 7\%$ decrease in SVR; $P < 0.05$). In CH rats, SIN-1 (i.c.v.) did not alter PVR, but it did decrease MPAP by $21 \pm 3\%$ ($P < 0.01$) owing to a $22 \pm 5\%$ decrease in CO ($P < 0.05$). Sydnominine-1 provoked a larger decrease in CO in CH rats ($22 \pm 5\%$ decrease; $P < 0.05$), so that the fall in MABP was also greater in CH rats ($46 \pm 3\%$ decrease), because the decline in SVR was similar for N rats and CH rats (27 ± 7 and 29% decrease in SVR, respectively).

In N rats, the CO response to acute hypoxia was depressed by SIN-1 so that, even though the MPAP response appeared to be unchanged (Fig. 2a), the PVR response to hypoxia was accentuated by SIN-1 (64 ± 24 and $127 \pm 26\%$ increase, respectively; Fig. 2b). Sydnominine-1 reduced the magnitude of the MABP and SVR responses to hypoxia, although the absolute MABP (and SVR)

values during hypoxia before and after SIN-1 were similar. In addition, SIN-1 abolished the small hypoxia-induced decline in HR observed prior to SIN-1 administration.

In CH rats, SIN-1 restored the pulmonary vasoconstriction in response to acute hypoxia. This was evident by a $33 \pm 5\%$ increase in MPAP (cf. a 3% increase for control) and a $90 \pm 11\%$ increase in PVR (cf. a 20% increase for control). The effect of SIN-1 on the MABP, SVR, CO and HR responses to acute hypoxia were similar for N and CH rats (Fig. 2a,b).

DISCUSSION

To date, this is the first study to investigate the central role of NO in: (i) modulating MPAP in the normal and hypertensive state; and (ii) acute HPV. The primary findings of the present study show that, in both N and CH rats, the acute central inhibition of NOS does not appear to modulate baseline MPAP or pulmonary vascular

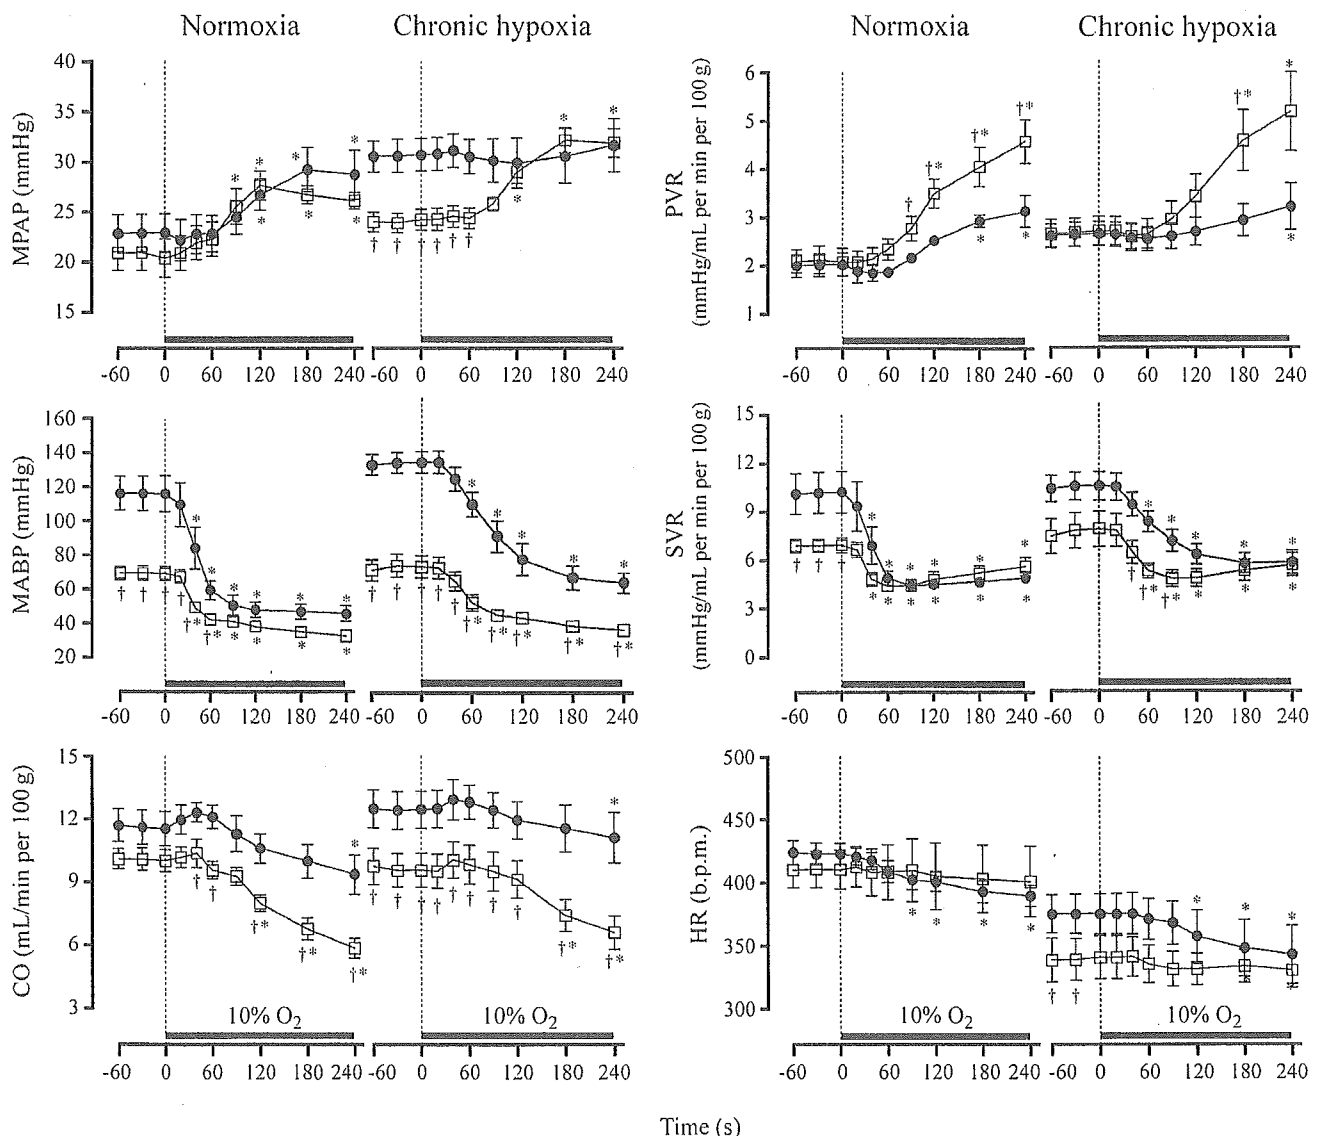


Fig. 2 Effect of i.c.v. sydnominine-1 (SIN-1) on mean pulmonary arterial pressure (MPAP), mean arterial blood pressure (MABP), cardiac output (CO), pulmonary vascular resistance (PVR), systemic vascular resistance (SVR) and heart rate (HR) responses to acute hypoxia ($10\% \text{O}_2$ for 4 min) in normoxic (N) rats ($n = 5$) and chronic hypoxic (CH) rats ($n = 6$). (●), control (artificial cerebrospinal fluid); (□), SIN-1 ($100 \mu\text{g}$ in $10 \mu\text{L}$). * $P < 0.05$ compared with pre-acute hypoxia values; † $P < 0.05$ compared with SIN-1-values.

Table 3 Steady state responses to intracerebroventricular syndnonimine-1 (100 µg in 10 µL) in normoxic rats (*n* = 5) and chronic-hypoxic rats (*n* = 6)

	Normoxia		Chronic hypoxia	
	Control	SIN-1	SIN-1	Control
MPAP (mmHg)	22.9 ± 1.7	20.8 ± 1.8	30.6 ± 1.6	24.1 ± 1.0*
MABP (mmHg)	116 ± 10	69 ± 4*	122 ± 6	67 ± 6**
CO (mL/min per 100 g)	11.64 ± 0.81	10.08 ± 0.51	12.46 ± 0.89	9.63 ± 0.81*
HR (b.p.m.)	423 ± 9	410 ± 15	375 ± 16	339 ± 17**
SVR (mmHg/mL per min per 100 g)	10.20 ± 1.28	6.93 ± 0.42*	10.07 ± 0.82	7.36 ± 1.06*
PVR (mmHg/mL per min per 100 g)	2.02 ± 0.23	2.10 ± 0.27	2.54 ± 0.24	2.58 ± 0.28

Data are the mean ± SEM. **P* < 0.05, ***P* < 0.01 compared with control values.

SIN-1, syndnonimine-1; MPAP, mean pulmonary arterial pressure; MABP, mean arterial blood pressure; CO, cardiac output; HR, heart rate; SVR, systemic vascular resistance; PVR, pulmonary vascular resistance.

reactivity to acute hypoxia. However, exogenous NO reduces baseline MPAP in CH rats, primarily by reducing CO, and enhances the HPV.

We demonstrated that exposure to 12% O₂ for 2 weeks induced pulmonary arterial hypertension, which concurs with numerous reports in the literature regarding the effects of CH on the pulmonary vasculature.^{6,29,30} Compared with the pulmonary vasculature, the systemic vasculature seems to be less affected by CH. We did not observe any difference in MABP between N and CH rats, which is similar to some reports.^{30,31} In contrast, Huang *et al.*⁶ did note an increase in MABP after 2 weeks of CH, although they described the increase in MABP as mild compared with the increase in MPAP.

The mechanisms responsible for the development of pulmonary hypertension remain poorly understood. Although a reduction in the local release of NO from the pulmonary endothelium has been implicated,^{5,8,32} Hampl *et al.*³⁰ reported that chronic inhibition of NOS did not increase MPAP, indicating that factors other than, or in addition to, a decrease in pulmonary NOS activity were responsible for the development of pulmonary hypertension. Furthermore, Weissmann *et al.*²⁷ investigated the role of pulmonary NO in the acute HPV response and concluded that attenuation of the acute HPV by chronic hypoxia preceded the development of pulmonary hypertension and was independent of the pulmonary endothelial NO system. Therefore, we hypothesized that disruption of the central NO pathways may contribute, at least in part, to the pathogenesis of pulmonary hypertension during chronic hypoxia.

Our results indicate that, using L-NAME, central NO has a minimal role, if any, in modulating tonic pulmonary vascular tone in the normal and hypertensive state. However, we cannot rule out the possibility that the dose of L-NAME selected in the present study did not completely inhibit NOS within the cardiovascular control centres. Preliminary experiments indicated that when L-NAME is injected i.v., doses above 150 µg had small direct systemic effects (similar preliminary experiments were conducted to determine the dose of SIN-1 with which to inject i.c.v. that did not directly alter pulmonary vasculature when injected i.v.). Therefore, because L-NAME can cross the blood-brain barrier,³³ we avoided higher doses of L-NAME that could have potentially directly modulated pulmonary vascular tone. Furthermore, a study by Nurminen *et al.*³⁴ reported that 30 µg L-NAME, i.c.v., provoked a significant increase in ABP that lasted for 10 min. Therefore, we were confident that a dose of 150 µg L-NAME would induce sufficient central NOS inhibition.

Although we found that L-NAME did not alter the acute HPV, we cannot exclude the possibility that the central actions of

L-NAME had fully subsided before testing acute hypoxia. However, preliminary experiments (data not shown) indicated that, even when L-NAME was administered immediately before the acute hypoxic test, the cardiovascular responses to acute hypoxia were not different to the responses prior to L-NAME. Alternatively, acute hypoxia is known to be a powerful activator of sympathetic nerve activity.³⁵ Because it has been well documented that the central administration of L-NAME increases sympathetic activity,^{36,37} it may be possible that, in the present study, L-NAME did not alter the HVR because sympathetic activity was already elevated by the acute hypoxic stimulus.

Although central L-NAME did not alter pulmonary vasculature tone, the intravenous administration of L-NAME did cause a small increase in PVR in N rats, which was accentuated after chronic hypoxia. Furthermore, the acute HVR was accentuated by L-NAME (i.v.) in both N and CH rats. Several studies have indicated that local endothelial NO has a limited role, if any, in the tonic modulation of MPAP,^{6,38} although Huang *et al.*⁶ indicated that local NO: (i) was more important in modulating pulmonary vasculature after chronic hypoxia; and (ii) was essential for maintaining low pulmonary resistance during acute hypoxia.

In comparison, the magnitude of the systemic vasoconstrictive response to L-NAME (i.v.) was substantially larger than that of the pulmonary vasculature. In agreement, several studies have indicated that local inhibition of NOS has an insignificant effect on tonic modulation of the pulmonary vasculature, but it is critical in modulating the systemic vasculature.^{6,30,38}

It has been well documented that central inhibition of NO increases MABP^{34,39,40} by increasing sympathetic nerve activity.^{36,37} We also reported that i.c.v. L-NAME provoked a significant increase in MABP, although one of the limitations of the present study is that we did not measure sympathetic activity. However, we found that the provoked increase in MABP by i.c.v. L-NAME in the normoxic rat was not accompanied by a baroreflex decrease in HR, which occurs when L-NAME is injected intravenously. Nurminen *et al.*³⁴ also reported that i.c.v. L-NAME caused a paradoxical increase in HR and, thus, concluded that the increase in HR was indirect evidence that L-NAME provoked an increase in sympathetic activity.

With regards to the pulmonary vasculature, an increase in sympathetic activity can cause either vasoconstriction (α-adreno-receptor mediated) or vasodilation (β-adreno-receptor mediated), depending on the initial pulmonary vascular tone.^{41,42} Therefore, assuming that i.c.v. L-NAME did increase pulmonary sympathetic activity, it is possible that we were unable to detect any change

in MPAP because of the potential opposing effects of α - and β -adrenoceptor activation within the pulmonary vasculature.

In the present study, as well as in other studies, the central administration of NO donors has been shown to reduce MABP.^{25,43} Nurminen and Vapaatalo⁴⁴ also showed that certain NO-releasing substances, such as nitroprusside, reduced MABP, although they also mentioned that the central administration of SIN-1 (approximately 600 $\mu\text{g}/\text{kg}$) increased MABP.

At high doses, SIN-1 can cogenerate NO and superoxide anions.^{45,46} Furthermore, an increase in the central generation of superoxide anions has been reported to increase sympathetic activity and, consequently, ABP.⁴⁷ Therefore, the increase in MABP in the study of Nurminen and Vapaatalo⁴⁴ may be attributed to the formation of superoxide anions. At low doses, the superoxide-associated effects of SIN-1 are significantly outweighed by the actions of NO.⁴⁵ Therefore, because the present study used a comparatively low dose of SIN-1 (100 μg), we interpret the decrease in MABP to indicate that, at this dose, SIN-1 was acting solely as an NO donor.

The decrease in MABP following the central administration of exogenous NO has been attributed to a decrease in sympathetic activity.^{40,48} To date, the present study is the first to investigate the effects of a central NO donor on MPAP. The important finding of the present study is that exogenous NO did not directly alter baseline pulmonary vascular tone (i.e. PVR was not altered), but it did enhance (in N rats) or restore (in CH rats) the acute HPV response. These results support the idea that central NO has little influence on the tonic modulation of pulmonary vascular tone, although it enhances the acute HPV.

Although we cannot confirm the underlying mechanisms responsible for these observations, it is possible that SIN-1 did reduce sympathetic activity in the rats in the present study, subsequently enhancing the HPV. Shirai *et al.*⁴⁹ demonstrated that β -adrenoceptor blockade had only a minor effect on baseline pulmonary vascular tone in normoxia, but it significantly accentuated the acute HPV (α -adrenoceptor blockade had no effect on the magnitude of the HPV). This observation may explain the reason as to why central SIN-1 did not affect baseline PVR but accentuated the HPV in the present study. Although PVR was not affected, central SIN-1 did reduce MPAP in the present study (significantly in CH rats), solely due to a reduction in CO. This, too, may be due to a reduction in β -adrenoceptor activity, because β -adrenoceptor attenuation has been reported to significantly reduce CO.^{50,51}

The mechanism(s) responsible for the attenuation of the HPV after chronic hypoxia remain poorly understood. However, it is possible to speculate that β -adrenoceptor upregulation may be one contributing factor because previous studies have shown that chronic hypoxia significantly increases β -adrenoceptor numbers within the lung.^{52,53} Changes in β -adrenoceptor availability during chronic hypoxia could potentially limit the development of pulmonary hypertension and, therefore, be physiologically beneficial; an important area that warrants further research.

In summary, we have shown that central NO has a limited role in modulating tonic MPAP in the normal and hypertensive states. However, exogenous NO enhanced the acute HPV, although central NO inhibition had no effect on the acute HPV. Whether central NO acts to inhibit β -adrenoceptor-mediated vasodilation of the acute HPV is another area that warrants further investigation. The present study used an anaesthetized preparation to investigate the

modulation of MPAP in normoxia and after chronic hypoxia. We did not, however, address any potential changes in the control of MPAP during the development of pulmonary hypertension. Hampl and Herget³⁸ indicated that, during the development of pulmonary hypertension, NO was essential in preventing pulmonary hypertension in the early stages, but became insignificant in the latter stages owing to endothelial dysfunction. Therefore, we will subsequently develop a conscious, chronically cannulated rat model to monitor the development of pulmonary hypertension during the chronic central inhibition/infusion of NO.

ACKNOWLEDGEMENT

The authors are very grateful for the aid and support provided by the Japan Society for the Promotion of Science (JSPS).

REFERENCES

1. Archer S, Rich S. Primary pulmonary hypertension: A vascular biology and translational research 'work in progress'. *Circulation* 2000; **102**: 2781–91.
2. Mandegar M, Yuan JX. Role of K^+ channels in pulmonary hypertension. *Vasc. Pharmacol.* 2002; **38**: 25–33.
3. Barbera JA, Peinado VI, Santos S. Pulmonary hypertension in COPD: Old and new concepts. *Monaldi Arch. Chest Dis.* 2000; **55**: 445–9.
4. Voelkel NF, Tudor RM. Hypoxia-induced pulmonary vascular remodeling: A model for what human disease? *J. Clin. Invest.* 2000; **106**: 733–8.
5. Fike CD, Kaplowitz MR, Thomas CJ, Nelin LD. Chronic hypoxia decreases nitric oxide production and endothelial nitric oxide synthase in newborn pig lungs. *Am. J. Physiol.* 1998; **274**: L517–26.
6. Huang KL, Wu CP, Kang BH, Lin YC. Chronic hypoxia attenuates nitric oxide-dependent hemodynamic responses to acute hypoxia. *J. Biomed. Sci.* 2002; **9**: 206–12.
7. Cornwell TL, Arnold E, Boerth NJ, Lincoln TM. Inhibition of smooth muscle cell growth by nitric oxide and activation of cAMP-dependent protein kinase by cGMP. *Am. J. Physiol.* 1994; **267**: C1405–13.
8. Le Cras TD, McMurtry IF. Nitric oxide production in the hypoxic lung. *Am. J. Physiol. Lung Cell. Mol. Physiol.* 2001; **280**: L575–82.
9. Sato J, Nair K, Hiddinga J *et al.* eNOS gene transfer to vascular smooth muscle cells inhibits cell proliferation via upregulation of p27 and p21 and not apoptosis. *Cardiovasc. Res.* 2000; **47**: 697–706.
10. Palmer RM, Rees DD, Ashton DS, Moncada S. L-Arginine is the physiological precursor for the formation of nitric oxide in endothelium-dependent relaxation. *Biochem. Biophys. Res. Commun.* 1988; **153**: 1251–6.
11. Fagan KA, Fouty BW, Tyler RC *et al.* The pulmonary circulation of homozygous or heterozygous eNOS-null mice is hyperresponsive to mild hypoxia. *J. Clin. Invest.* 1999; **103**: 291–9.
12. Steudel W, Ichinose F, Huang PL *et al.* Pulmonary vasoconstriction and hypertension in mice with targeted disruption of the endothelial nitric oxide synthase (NOS 3) gene. *Circ. Res.* 1997; **81**: 34–41.
13. Steudel W, Scherrer-Crosbie M, Bloch KD *et al.* Sustained pulmonary hypertension and right ventricular hypertrophy after chronic hypoxia in mice with congenital deficiency of nitric oxide synthase 3. *J. Clin. Invest.* 1998; **101**: 2468–77.
14. Ozaki M, Kawashima S, Yamashita T *et al.* Reduced hypoxic pulmonary vascular remodeling by nitric oxide from the endothelium. *Hypertension* 2001; **37**: 322–7.
15. Sato K, Rodman DM, McMurtry IF. Hypoxia inhibits increased ET_B receptor-mediated NO synthesis in hypertensive rat lungs. *Am. J. Physiol.* 1999; **276**: L571–81.
16. Xue C, Rengasamy A, Le Cras TD, Koberna PA, Dailey GC, Johns RA. Distribution of NOS in normoxic vs. Hypoxic rat lung:

- Upregulation of NOS by chronic hypoxia. *Am. J. Physiol.* 1994; **267**: L667–78.
17. Shirai M, Pearson JT, Shimouchi A *et al.* Changes in functional and histological distributions of nitric oxide synthase caused by chronic hypoxia in rat small pulmonary arteries. *Br. J. Pharmacol.* 2003; **139**: 899–910.
 18. Le Cras TD, Xue C, Rengasamy A, Johns RA. Chronic hypoxia upregulates endothelial and inducible NO synthase gene and protein expression in rat lung. *Am. J. Physiol.* 1996; **270**: L164–70.
 19. Matsumura K, Tsuchihashi T, Kagiya S, Abe I, Fujishima M. Role of nitric oxide in the nucleus of the solitary tract of rats. *Brain Res.* 1998; **798**: 232–8.
 20. Zanzinger J, Czachurski J, Sellar H. Inhibition of basal and reflex-mediated sympathetic activity in the RVLM by nitric oxide. *Am. J. Physiol.* 1995; **268**: R958–62.
 21. Ohta A, Takagi H, Matsui T, Hamai Y, Iida S, Esumi H. Localization of nitric oxide synthase-immunoreactive neurons in the solitary nucleus and ventrolateral medulla oblongata of the rat: Their relation to catecholaminergic neurons. *Neurosci. Lett.* 1993; **158**: 33–5.
 22. Garthwaite J, Boulton CL. Nitric oxide signaling in the central nervous system. *Annu. Rev. Physiol.* 1995; **57**: 683–706.
 23. Patel KP, Li YF, Hirooka Y. Role of nitric oxide in central sympathetic outflow. *Exp. Biol. Med.* 2001; **226**: 814–24.
 24. Hironaga K, Hirooka Y, Matsuo I *et al.* Role of endogenous nitric oxide in the brain stem on the rapid adaptation of baroreflex. *Hypertension* 1998; **31**: 27–31.
 25. Nishimura M, Takahashi H, Nanbu A, Sakamoto M, Yoshimura M. Cardiovascular regulation by L-arginine in the brain of rats: Role of the brain renin-angiotensin system and nitric oxide. *Am. J. Hypertens.* 1997; **10**: 389–96.
 26. Clini E, Ambrosino N. Nitric oxide and pulmonary circulation. *Med. Sci. Monit.* 2002; **8**: RA178–82.
 27. Weissmann N, Nollen M, Gerigk B *et al.* Downregulation of hypoxic vasoconstriction by chronic hypoxia in rabbits: Effects of nitric oxide. *Am. J. Physiol. Heart Circ. Physiol.* 2003; **284**: H931–8.
 28. Paxinos G, Watson C. *The Brain in Stereotaxic Coordinates*, 4th edn. Academic Press, San Diego, CA. 1998.
 29. Ao Q, Huang L, Zhu P, Xiong M, Wang D. Inhibition of expression of hypoxia-inducible factor-1 α mRNA by nitric oxide in hypoxic pulmonary hypertension rats. *J. Huazhong Univ. Sci. Technol. Med. Sci.* 2004; **24**: 5–8.
 30. Hampl V, Archer SL, Nelson DP, Weir EK. Chronic EDRF inhibition and hypoxia: Effects on pulmonary circulation and systemic blood pressure. *J. Appl. Physiol.* 1993; **75**: 1748–57.
 31. Coney AM, Bishay M, Marshall JM. Influence of endogenous nitric oxide on sympathetic vasoconstriction in normoxia, acute and chronic systemic hypoxia in the rat. *J. Physiol.* 2004; **555**: 793–804.
 32. Adnot S, Raffestin B, Eddahibi S, Braquet P, Chabrie PE. Loss of endothelium-dependent relaxant activity in the pulmonary circulation of rats exposed to chronic hypoxia. *J. Clin. Invest.* 1991; **87**: 155–62.
 33. Bansinath M, Arbabha B, Turndorf H, Garg UC. Chronic administration of a nitric oxide synthase inhibitor N-nitro-L-arginine, and drug-induced increase in cerebellar cyclic GMP *in vivo*. *Neurochem. Res.* 1993; **18**: 1063–6.
 34. Nurminen ML, Ylikorkala A, Vapaatalo H. Central inhibition of nitric oxide synthesis increases blood pressure and heart rate in anesthetized rats. *Methods Fundam. Exp. Clin. Pharmacol.* 1997; **19**: 35–41.
 35. Fletcher EC. Invited review: Physiological consequences of intermittent hypoxia: Systemic blood pressure. *J. Appl. Physiol.* 2001; **90**: 1600–5.
 36. Harada S, Tokunaga S, Momohara M *et al.* Inhibition of nitric oxide formation in the nucleus tractus solitarius increases renal sympathetic nerve activity in rabbits. *Circ. Res.* 1993; **72**: 511–16.
 37. Zanzinger J, Czachurski J, Sellar H. Nitric oxide in the ventrolateral medulla regulates sympathetic responses to systemic hypoxia in pigs. *Am. J. Physiol.* 1998; **275**: R33–9.
 38. Hampl V, Herget J. Role of nitric oxide in the pathogenesis of chronic pulmonary hypertension. *Physiol. Rev.* 2000; **80**: 1337–72.
 39. Choi KC, Jung M, Lee JU, Kim SW, Kim NH, Kang YJ. Attenuated central pressor response to nitric oxide synthesis inhibition in chronic renal failure rats. *Korean J. Intern. Med.* 1997; **12**: 58–61.
 40. Togashi H, Sakuma I, Yoshioka M *et al.* A central nervous system action of nitric oxide in blood pressure regulation. *J. Pharmacol. Exp. Ther.* 1992; **262**: 343–7.
 41. Shirai M, Shindo T, Shimouchi A, Ninomiya I. Diameter and flow velocity changes of feline small pulmonary vessels in response to sympathetic nerve stimulation. *Pflügers Arch.* 1994; **429**: 267–73.
 42. Shirai M, Matsukawa K, Nishiura N, Kawaguchi AT, Ninomiya I. Changes in efferent pulmonary sympathetic nerve activity during systemic hypoxia in anesthetized cats. *Am. J. Physiol.* 1995; **269**: R1404–9.
 43. Matsumura K, Abe I, Tsuchihashi T, Fujishima M. Central nitric oxide attenuates the baroreceptor reflex in conscious rabbits. *Am. J. Physiol.* 1998; **274**: R1142–9.
 44. Nurminen ML, Vapaatalo H. Effect of intracerebroventricular and intravenous administration of nitric oxide donors on blood pressure and heart rate in anaesthetized rats. *Br. J. Pharmacol.* 1996; **119**: 1422–6.
 45. Stopper H, Moller M, Bommel HM, Schmidt HH. Cytotoxic versus genotoxic effects of nitric oxide (NO). *Toxicol. Lett.* 1999; **106**: 59–67.
 46. Megson IL, Webb DJ. Nitric oxide donor drugs: Current status and future trends. *Expert Opin. Investig. Drugs* 2002; **11**: 587–601.
 47. Gao L, Wang W, Li YL *et al.* Superoxide mediates sympathoexcitation in heart failure: Roles of angiotensin II and NAD(P)H oxidase. *Circ. Res.* 2004; **95**: 937–44.
 48. Shapoval LN, Sagach VF, Pobegailo LS. Nitric oxide influences ventrolateral medullary mechanisms of vasomotor control in the cat. *Neurosci. Lett.* 1991; **132**: 47–50.
 49. Shirai M, Shindo T, Ninomiya I. β -Adrenergic mechanisms attenuated hypoxic pulmonary vasoconstriction during systemic hypoxia in cats. *Am. J. Physiol.* 1994; **266**: H1777–85.
 50. Kontos HA, Lower RR. Role of beta-adrenergic receptors in the circulatory response to hypoxia. *Am. J. Physiol.* 1969; **217**: 756–63.
 51. Chiong MA, Hatcher JD. The sympathoadrenergic system in the cardiovascular responses to hypoxia in the dog. *Can. J. Physiol. Pharmacol.* 1972; **50**: 674–83.
 52. Birnkrant DJ, Davis PB, Ernsberger P. Visualization of high- and low-affinity beta-adrenergic receptors in rat lung: Upregulation by chronic hypoxia. *Am. J. Physiol.* 1993; **265**: L389–94.
 53. Winter RJ, Dickinson KE, Rudd RM, Sever PS. Tissue specific modulation of beta-adrenoceptor number in rats with chronic hypoxia with an attenuated response to down-regulation by salbutamol. *Clin. Sci.* 1986; **70**: 159–65.

X-ray Spectra from a Characteristic X-ray Generator with a Molybdenum Tube

Eiichi Sato^a, Etsuro Tanaka^b, Hidezo Mori^c, Toshiaki Kawai^d, Takashi Inoue^e,
Akira Ogawa^e, Kiyomi Takahashi^f, Shigehiro Sato^f and Kazuyoshi Takayama^g

(Received October 31, 2005)

Abstract

This generator consists of the following components: a constant high-voltage power supply, a filament power supply, a turbomolecular pump, and an x-ray tube. The x-ray tube is a demountable diode which is connected to the turbomolecular pump and consists of the following major devices: a molybdenum rod target, a tungsten hairpin cathode (filament), a focusing electrode, a polyethylene terephthalate x-ray window 0.25 mm in thickness, and a stainless-steel tube body. In the x-ray tube, the positive high voltage is applied to the anode (target) electrode, and the cathode is connected to the tube body (ground potential). In this experiment, the tube voltage applied was from 22 to 36 kV, and the tube current was regulated to within 100 μ A by the filament temperature. The exposure time is controlled in order to obtain optimum x-ray intensity. The electron beams from the cathode are converged to the target by the focusing electrode, and x-rays are produced through the focusing electrode. Using a lithium fluoride curved crystal, clean K-series characteristic x-rays were observed without using a filter. However, bremsstrahlung x-rays were observed using a cadmium telluride detector.

Keywords: demountable x-ray tube, quasi-monochromatic x-rays, K-series characteristic x-rays, Sommerfeld's theory, curved crystal, cadmium telluride detector

1. Introduction

Most flash x-ray generators employ high-voltage condensers and cold-cathode x-ray tubes,^{1,5} and the plasma x-ray source has been growing with increases in the electrostatic energy in the condenser. By

^a Department of Physics, Iwate Medical University, 3-16-1 Honchodori, Morioka 020-0015, Japan

^b Department of Nutritional Science, Faculty of Applied Bio-science, Tokyo University of Agriculture, 1-1-1 Sakuragaoka, Setagaya-ku 156-8502, Japan

^c Department of Cardiac Physiology, National Cardiovascular Center Research Institute, 5-7-1 Fujishirodai, Suita, Osaka 565-8565, Japan

^d Electron Tube Division #2, Hamamatsu Photonics K. K., 314-5 Shimokanzo, Iwata 438-0193, Japan

^e Department of Neurosurgery, School of Medicine, Iwate Medical University, 19-1 Uchimaru, Morioka 020-8505, Japan

^f Department of Microbiology, School of Medicine, Iwate Medical University, 19-1 Uchimaru, Morioka 020-8505, Japan

^g Shock Wave Research Center, Institute of Fluid Science, Tohoku University, 2-1-1 Katahira, Sendai 980-8577, Japan

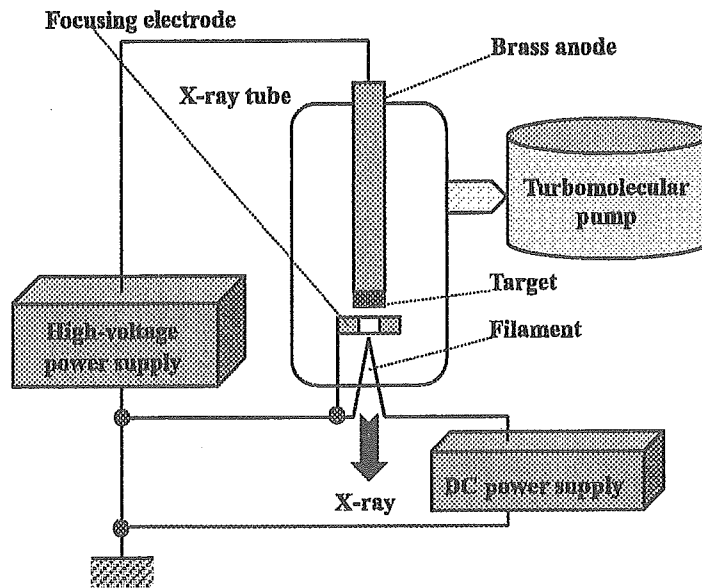


Fig. 1: Block diagram including the main transmission line of the compact x-ray generator with a quasi-monochromatic diode.

forming weakly ionized linear plasma⁶⁻⁹ using a rod-target triode, we confirmed irradiation of clean K-series characteristic x-rays such as hard x-ray lasers and their higher harmonic hard x-rays from the plasma axial direction. Because the plasma transmits high-photon-energy bremsstrahlung x-rays, it is difficult to produce high-photon-energy characteristic x-rays. In view of this situation, we have developed a super-fluorescent x-ray generator¹⁰⁻¹³ by forming weakly ionized plasma at the target tip and have succeeded in producing comparatively clean K-series characteristic x-rays of molybdenum, cerium, tantalum, and tungsten. In particular, the cerium target is useful for performing iodine K-edge angiography, and gadolinium K-edge angiography can be performed using tantalum and tungsten targets.

Steady-state K-series characteristic x-rays left by filters have been employed to perform mammography using a molybdenum target and to perform K-edge angiography¹⁴⁻¹⁷ using a cerium target. In addition, the rays are also useful for performing real-time radiography achieved with a flat panel detector. Because the characteristic x-ray intensity decreases with increases in the filter thickness, the development of a characteristic x-ray generator utilizing the angle dependence of bremsstrahlung x-rays has been wished for.

In the spectrum measurements, we employ a cadmium telluride detector and a lithium fluoride curved crystal. The detector is useful to measure the total spectra including scattering beams. On the other hand, the spectra from only the x-ray source can be measured using the crystal by selecting Bragg's angle.

In this paper, we describe an x-ray generator developed and used to perform a preliminary experiment for generating clean K-series characteristic x-rays by angle dependence of the bremsstrahlung x-rays and measurement of the x-ray spectra using two methods.