

### 3. CHARACTERISTICS

#### 3.1 X-ray intensity

The x-ray intensity was measured by a Victoreen 660 ionization chamber at 1.0 m from the x-ray source using a 50- $\mu\text{m}$ -thick tungsten filter (Fig. 3). At a constant tube current, the x-ray intensity increased when the tube voltage was increased. At a tube voltage of 60 kV and a current of 0.10 mA, the intensity with the filter was 1.04  $\mu\text{Gy/s}$ .

#### 3.2 Focal spot

In order to measure images of the x-ray source, we employed a pinhole camera with a hole diameter of 100  $\mu\text{m}$  in conjunction with a Computed Radiography (CR) system with a sampling pitch of 87.5  $\mu\text{m}$  (Fig. 4). When the tube voltage was increased using the filter, the spot diameter increased and had a maximum value of approximately 2.2 mm with a tube voltage of 70 kV.

#### 3.3 X-ray spectra

In order to measure x-ray spectra, we employed a cadmium telluride detector (XR-100T, Amptek) (Fig. 5). Using the filter, low-photon-energy bremsstrahlung x-rays were absorbed, and sharp K lines were left. When the tube voltage was increased, the x-ray intensities of samarium K-series characteristic lines increased, and the maximum photon energy increased.

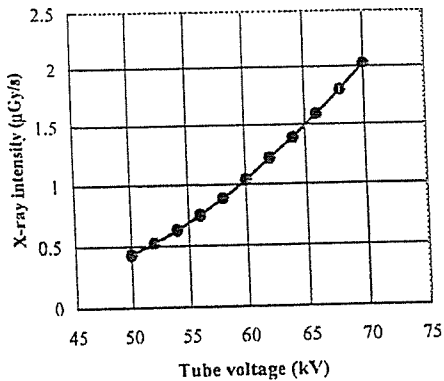


Fig. 3. X-ray intensity measured at 1.0 m from X-ray source according to changes in tube voltage using a tungsten filter.

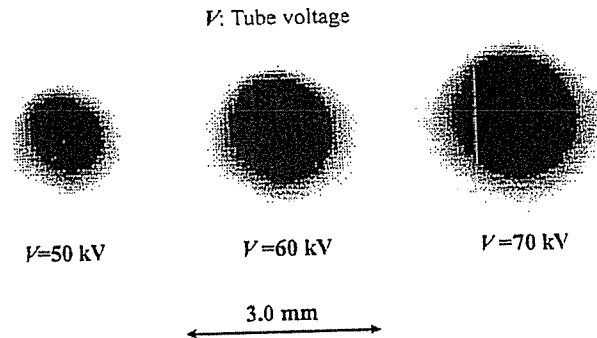


Fig. 4. Images of the x-ray source with changing the tube voltage.

### 4. K-EDGE ANGIOGRAPHY

Because the average photon energy of samarium  $K\alpha$  is 39.9 keV, iodine contrast media with a K-absorption edge of 33.2 keV absorb the  $K\alpha$  lines easily (Fig. 6). Therefore, blood vessels were observed with high contrasts. The angiography was performed using the CR system, iodine microspheres of 15  $\mu\text{m}$  in diameter, and the filter. The distance between the x-ray source and the imaging plate was 1.0 m, and the tube voltage was 60 kV. First, rough measurements of spatial resolution were made using wires coiled around rods made of polymethyl methacrylate (PMMA) (Fig. 7). Although the image contrast decreased somewhat with decreases in the wire diameter, a 50- $\mu\text{m}$ -diameter wire could be observed. Figures 8 and 9 show angiograms of a rabbit heart and thigh, respectively. The coronary arteries in the heart and fine blood vessels in the thigh were visible. Figure 10 shows angiograms of a dog heart, and blood vessels of approximately 100  $\mu\text{m}$  in diameter were observed.

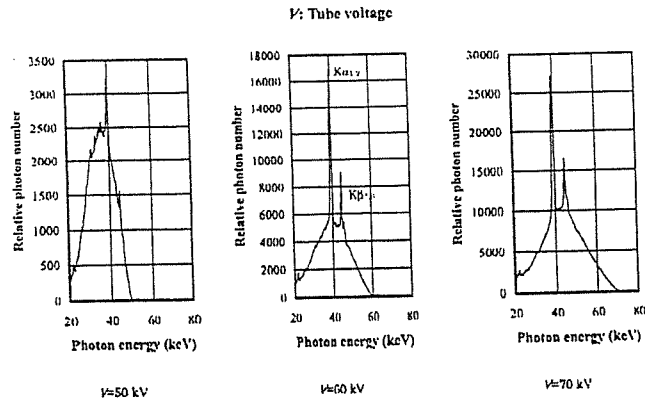


Fig. 5. X-ray spectra measured using a cadmium telluride detector with changes in tube voltage using the filter.

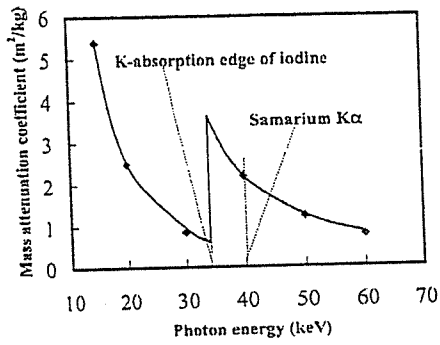


Fig. 6. Mass attenuation coefficients of iodine and average photon energy of samarium  $K\alpha$  lines.

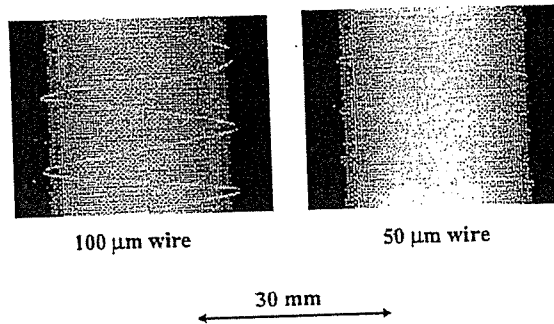


Fig. 7. Radiograms of tungsten wires coiled around PMMA rods.

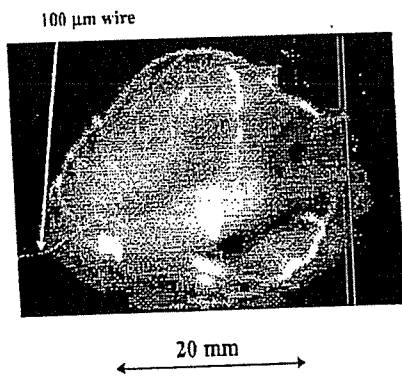


Fig. 8. Angiograms of an extracted rabbit heart using iodine microspheres.

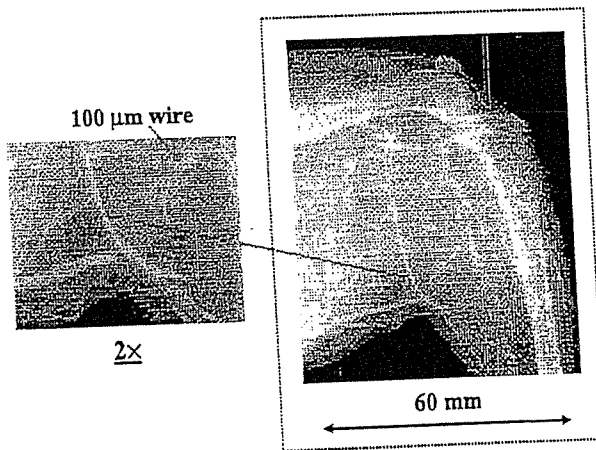


Fig. 9. Angiogram of a rabbit thigh using iodine microspheres.

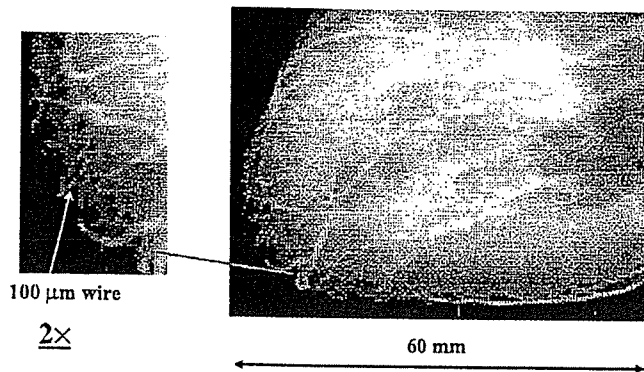


Fig. 10. Angiogram of an extracted dog heart using iodine microspheres.

## 5. DISCUSSION AND CONCLUSIONS

We employed an x-ray generator with a samarium-target tube and succeeded in producing samarium characteristic x-rays, which can be absorbed easily by iodine-based contrast media. Both the characteristic and bremsstrahlung x-ray intensities increased with increases in the tube voltage without filtering. Using the filter, K-rays were left by absorbing bremsstrahlung rays, and K-ray intensity increased with increases in the tube voltage.

Using this x-ray tube, we could produce K-series characteristic x-rays of nickel, copper, and molybdenum, and performed soft radiography. However it is difficult to produce clean samarium K-rays because bremsstrahlung x-ray intensity is in proportion to the atomic number. Therefore, optimum filters for absorbing bremsstrahlung rays should be employed to improve the image contrast of blood vessels.

Using the filter, the generator produced maximum number of characteristic photons was approximately  $4 \times 10^6$  photons/( $\text{cm}^2 \cdot \text{s}$ ) at 1.0 m from the source, and the photon count rate can be increased easily by improving the target. For example, the rotation anode tube can be developed, and sufficient x-ray dose rates could be produced by increasing the anode diameter.

## ACKNOWLEDGMENT

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, and 16591222) and Advanced Medical Scientific Research from MECSST, Health and Labor Sciences Research Grants (RAMT-nano-001, RHGTEFB-genome-005 and RHGTEFB-saisei-003), and grants from the Keiryō Research Foundation, Promotion and Mutual Aid Corporation for Private Schools of Japan, Japan Science and Technology Agency (JST), and New Energy and Industrial Technology Development Organization (NEDO, Industrial Technology Research Grant Program in '03).

## REFERENCES

1. H. Mori, K. Hyodo, E. Tanaka, M. U. Mohammed, A. Yamakawa, Y. Shinozaki, H. Nakazawa, Y. Tanaka, T. Sekka, Y. Iwata, S. Honda, K. Umetani, H. Ueki, T. Yokoyama, K. Tanioka, M. Kubota, H. Hosaka, N. Ishizawa and M. Ando, "Small-vessel radiography in situ with monochromatic synchrotron radiation," *Radiology*, 201, 173-177, 1996.
2. K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita and J. Tada, "Development of a two-dimensional imaging system for clinical applications of intravenous coronary angiography using intense synchrotron radiation produced by a multipole wiggler," *J. Synchrotron Radiat.*, 5, 1123-1126, 1998.
3. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing weakly ionized linear copper plasma," *Rev. Sci. Instrum.*, 74,

5236-5240, 2003.

4. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Sharp characteristic x-ray irradiation from weakly ionized linear plasma," *J. Electron Spectrosc. Related Phenom.*, **137-140**, 713-720, 2004.
5. E. Sato, E. Tanaka, H. Mori, T. Kawai, S. Sato and K. Takayama, "Clean monochromatic x-ray irradiation from weakly ionized linear copper plasma," *Opt. Eng.*, **44**, 049002-1-6, 2005.
6. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Inoue, A. Ogawa, S. Sato, K. Takayama, J. Onagawa, "X-ray spectra from weakly ionized linear copper plasma," *Jpn. J. Appl. Phys.*, **45**, 5301-5306, 2006.
7. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Inoue, A. Ogawa, S. Sato, K. Takayama and J. Onagawa, "Characteristic x-ray generator utilizing angle dependence of bremsstrahlung x-ray distribution," *Jpn. J. Appl. Phys.*, **45**, 2845-2849, 2006.
8. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Demonstration of enhanced K-edge angiography using a cerium target x-ray generator," *Med. Phys.*, **31**, 3017-3021, 2004.
9. E. Sato, A. Yamadera, E. Tanaka, H. Mori, T. Kawai, F. Ito, T. Inoue, A. Ogawa, S. Sato, K. Takayama, J. Onagawa and H. Ido, "X-ray spectra from a cerium target and their application to cone beam K-edge angiography," *Opt. Eng.*, **44**, 096502-1-6, 2005.
10. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Inoue, A. Ogawa, A. Yamadera, S. Sato, F. Ito, K. Takayama, J. Onagawa and H. Ido, "Variations in cerium x-ray spectra and enhanced K-edge angiography," *Jpn. J. Appl. Phys.*, **44**, 8204-8209, 2005.
11. E. Sato, K. Sato and Y. Tamakawa, "Film-less computed radiography system for high-speed imaging," *Ann. Rep. Iwate Med. Univ. Sch. Lib. Arts and Sci.*, **35**, 13-23, 2000.

\*dresato@iwate-med.ac.jp; phone +81-19-651-5111; fax +81-19-654-9282

# Enhanced real-time magnification angiography utilizing a 100- $\mu$ m-focus x-ray generator in conjunction with an image intensifier

Eiichi Sato<sup>\*a</sup>, Etsuro Tanaka<sup>b</sup>, Hidezo Mori<sup>c</sup>, Toshiaki Kawai<sup>d</sup>, Takashi Inoue<sup>e</sup>, Akira Ogawa<sup>e</sup>,  
Mitsuru Izumisawa<sup>f</sup>, Kiyomi Takahashi<sup>g</sup>, Shigehiro Sato<sup>g</sup>, Toshio Ichimaru<sup>h</sup>  
and Kazuyoshi Takayama<sup>i</sup>

<sup>a</sup>Department of Physics, Iwate Medical University, 3-16-1 Honchodori, Morioka 020-0015, Japan

<sup>b</sup>Department of Nutritional Science, Faculty of Applied Bio-science, Tokyo University of  
Agriculture, 1-1-1 Sakuragaoka, Setagaya-ku 156-8502, Japan

<sup>c</sup>Department of Cardiac Physiology, National Cardiovascular Center Research Institute, 5-7-1  
Fujishiro dai, Suita, Osaka 565-8565 Japan

<sup>d</sup>Electron Tube Division #2, Hamamatsu Photonics K.K., 314-5 Shimokanzo, Iwata 438-0193,  
Japan

<sup>e</sup>Department of Neurosurgery, School of Medicine, Iwate Medical University, 19-1 Uchimarui,  
Morioka 020-8505, Japan

<sup>f</sup>Department of Oral Radiology, School of Dentistry, Iwate Medical University, 1-3-27 Chuo,  
Morioka 020-0021, Japan,

<sup>g</sup>Department of Microbiology, School of Medicine, Iwate Medical University, 19-1 Uchimarui,  
Morioka 020-8505, Japan

<sup>h</sup>Department of Radiological Technology, School of Health Sciences, Hirosaki University, 66-1  
Honcho, Hirosaki 036-8564, Japan

<sup>i</sup>Tohoku University Biomedical Engineering Research Organization, Tohoku University, 2-1-1  
Katahira, Sendai 980-8577, Japan

## ABSTRACT

A microfocus x-ray tube is useful in order to perform magnification digital radiography including phase-contrast effect. The 100- $\mu$ m-focus x-ray generator consists of a main controller for regulating the tube voltage and current and a tube unit, with a high-voltage circuit and a fixed anode x-ray tube. The maximum tube voltage, current, and electric power were 105 kV, 0.5 mA, and 50 W, respectively. Using a 3.0-mm-thick aluminum filter, the x-ray intensity was 26.0  $\mu$ Gy/s at 1.0 m from the source with a tube voltage of 60 kV and a current of 0.50 mA. Because the peak photon energy was approximately 35 keV using the filter with a tube voltage of 60 kV, the bremsstrahlung x-rays were absorbed effectively by iodine-based contrast media with an iodine K-edge of 33.2 keV. Real-time magnification radiography was performed by twofold magnification imaging with an image intensifier camera, and angiography was achieved with iodine-based microspheres 15  $\mu$ m in diameter. In angiography of non-living animals, we observed fine blood vessels of approximately 100  $\mu$ m with high contrasts.

**Keywords:** real-time magnification radiography, magnification angiography, 100- $\mu$ m-focus tube, tungsten target, image intensifier, phase-contrast effect

## 1. INTRODUCTION

To perform high-speed biomedical radiography, several various flash x-ray generators using cold-cathode tubes have

Hard X-Ray and Gamma-Ray Detector Physics and Penetrating Radiation Systems VIII,  
edited by Larry A. Franks, Arnold Burger, Ralph B. James, H. Bradford Barber, F. Patrick Doty, Hans Roehrig,  
Proc. of SPIE Vol. 6319, 63190J, (2006) · 0277-786X/06/\$15 · doi: 10.1117/12.679220

Proc. of SPIE Vol. 6319 63190J-1

been developed.<sup>1-4</sup> In particular, quasi-monochromatic flash x-ray generators<sup>5-10</sup> have been designed to perform preliminary experiments for producing clean K-series x-rays, and higher-harmonic hard x-rays have been observed in a weakly ionized linear plasma of copper and nickel. However, in monochromatic flash radiography, difficulties in increasing x-ray duration and in performing x-ray computed tomography (CT) have been encountered. In view of this situation, we have developed steady-state characteristic x-ray generators to produce clean characteristic x-rays, since bremsstrahlung rays are not emitted in the opposite direction to that of electron trajectory.

Monochromatic parallel beams produced from a synchrotron using silicon crystals have been employed in phase-contrast radiography<sup>11,12</sup> and enhanced K-edge angiography.<sup>13,14</sup> In particular, the parallel beams with photon energies of approximately 35 keV have been employed to perform iodine K-edge angiography, because the beams are absorbed effectively by iodine-based contrast media with a K-absorption edge of 33.2 keV.

Without using synchrotrons, phase-contrast radiography for edge enhancement can be performed using a microfocus x-ray tube, and the magnification radiography including the phase-contrast effect<sup>15</sup> has been applied in mammography achieved with a computed radiography (CR) system<sup>16</sup> (Regius 190, Konica Minolta) with a sampling pitch of 43.8  $\mu\text{m}$  using a 100- $\mu\text{m}$ -focus molybdenum tube. Subsequently, we have developed a cerium x-ray generator<sup>17-19</sup> to perform enhanced K-edge angiography using cone beams, and have succeeded in observing fine blood vessels and coronary arteries with high contrasts using cerium K $\alpha$  rays of 34.6 keV. However, it is difficult to design a small focus cerium tube for angiography.

Magnification radiography is useful in order to improve the spatial resolution in digital radiography, and narrow photon energy bremsstrahlung x-rays with a peak energy of approximately 35 keV from a microfocus tungsten tube are useful to perform high-contrast high-resolution angiography. In magnification radiography, scattering beams from radiographic objects can be reduced without using a grid.

In this research, we employed a 100- $\mu\text{m}$ -focus tungsten tube, used to perform real-time magnification radiography, including angiography, using an image intensifier (II) in conjunction with a CCD camera.

## 2. X-RAY GENERATOR

Figure 1 shows the block diagram of a microfocus x-ray generator used in this experiment, and the generator consists of a main controller, an x-ray tube unit with a Cockcroft-Walton circuit, an insulation transformer, and a 100- $\mu\text{m}$ -focus x-ray tube. The tube voltage, the current, and the exposure time can be controlled by the controller. The main circuit for producing x-rays employs the Cockcroft-Walton circuit in order to decrease the dimensions of the tube unit. In the x-ray tube, the positive and negative high voltages are applied to the anode and cathode electrodes, respectively. The filament heating current is supplied by an AC power supply in the controller in conjunction with an insulation transformer which is used for isolation from the high voltage from the Cockcroft-Walton circuit. In this experiment, the tube voltage applied was from 45 to 70 kV, and the tube current was regulated to within 0.50 mA (maximum current) by the filament temperature. The exposure time is controlled in order to obtain optimum x-ray intensity, and narrow-photon-energy bremsstrahlung x-rays are produced using a 3.0-mm-thick aluminum filter for absorbing soft x-rays.

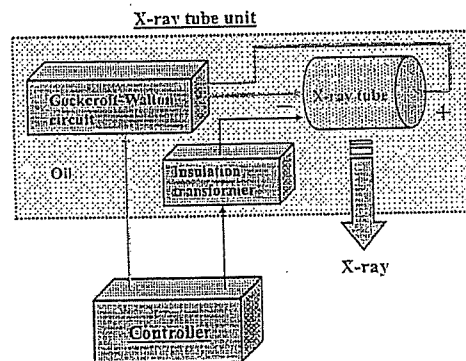


Fig. 1. Block diagram of the x-ray generator.

### 3. RESULTS AND DISCUSSION

#### 3.1 X-ray intensity

The x-ray intensity was measured by a Victoreen 660 ionization chamber at 1.0 m from the x-ray source using the filter (Fig. 2). At a constant tube current of 0.50 mA, the x-ray intensity increased when the tube voltage was increased. At a tube voltage of 60 kV, the intensity with the filter was 26.0  $\mu\text{Gy/s}$ .

#### 3.2 X-ray Spectra

In order to measure x-ray spectra, we employed a cadmium telluride detector (XR-100T, Amptek) (Fig. 3). When the tube voltage was increased, the bremsstrahlung x-ray intensity increased, and both the maximum photon energy and the spectrum peak energy increased.

In order to perform K-edge angiography, bremsstrahlung x-rays of approximately 35 keV are useful, and the high-energy bremsstrahlung x-rays decrease the image contrast. Using this filter, because bremsstrahlung x-rays with energies higher than 60 keV were not absorbed easily, the tube voltage for angiography was determined as 60 kV by considering the filtering effect of radiographic objects.

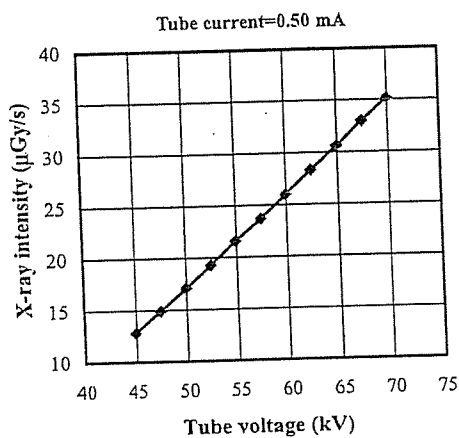


Fig. 2. X-ray intensity ( $\mu\text{Gy/s}$ ) as a function of tube voltage (kV) with a tube current of 0.50 mA.

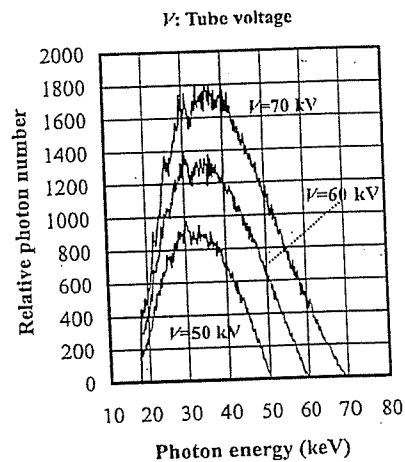


Fig. 3. Bremsstrahlung x-ray spectra measured using a cadmium telluride detector with changes in the tube voltage.

#### 3.3 Magnification radiography

The magnification radiography was performed by twofold magnification imaging using the II camera and the filter at a tube voltage of 60 kV, and the distance between the x-ray source and the II was 1.0 m (Figs. 4 and 5). First, the spatial resolution of magnification radiography was made using a lead test chart (Fig. 6). In the magnification radiography, 109  $\mu\text{m}$  lines (4.6 line pairs/mm) were visible. Subsequently, radiography of tungsten wires coiled around rods made of polymethyl methacrylate (PMMA) was performed (Fig. 7). Although the image contrast decreased somewhat with decreases in the wire diameter, a 50- $\mu\text{m}$ -diameter wire could be observed.

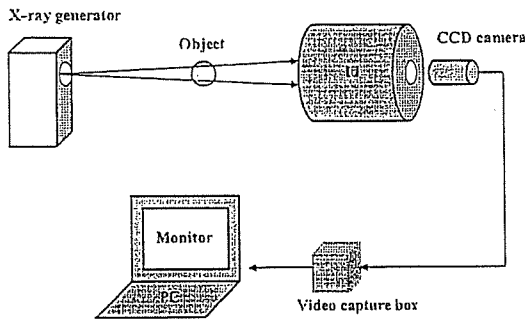


Fig. 4. Real-time magnification imaging using an image intensifier camera (low-resolution mode) in conjunction with a microfocus tube.

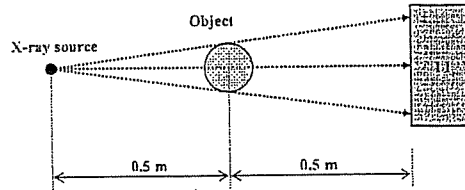


Fig. 5. Twofold magnification imaging.

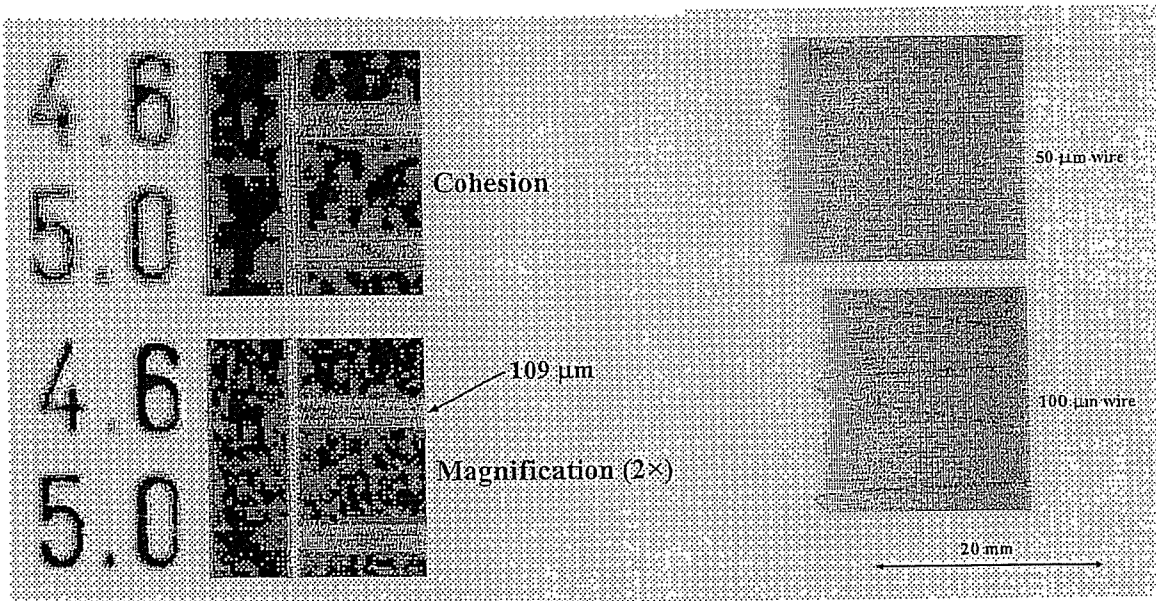


Fig. 6. Radiograms of a test chart for measuring the spatial resolution.

Fig. 7. Radiograms of tungsten wires coiled around PMMA rods.

### 3.4 Enhanced magnification angiography

Figure 8 shows the mass attenuation coefficients of iodine at the selected energies; the coefficient curve is discontinuous at the iodine K-edge. The effective bremsstrahlung x-ray spectra for K-edge angiography are shown above the iodine K-edge. Because iodine contrast media with a K-absorption edge of 33.2 keV absorb the rays easily, blood vessels were observed with high contrasts.

The magnification angiography was performed at the same conditions using iodine microspheres of 15 μm in diameter, and the microspheres (containing 37% iodine by weight) are very useful for making phantoms of non-living animals used for angiography. Angiograms of a rabbit heart on the turn table is shown in Fig. 9, and the coronary arteries are visible. Figure 10 shows angiograms of a dog heart in an xy table, and blood vessels of approximately 100 μm in diameter were observed.



#### 4. CONCLUSION AND OUTLOOK

We employed an x-ray generator with a 100- $\mu\text{m}$ -focus tungsten tube and performed real-time magnification radiography (fluoroscopy) using the II camera. To perform angiography, we employed narrow-photon-energy bremsstrahlung x-rays with a peak photon energy of approximately 35 keV, which can be absorbed easily by iodine-based contrast media. The bremsstrahlung x-ray intensity substantially increased with increases in the tube voltage, and the tube voltage was determined as 60 kV in order to increase the image contrast by decreasing high-photon-energy bremsstrahlung x-rays with energies beyond 60 keV. In enhanced angiography, low-photon-energy bremsstrahlung rays should be absorbed by an aluminum filter. Although we obtained mostly absorption-contrast images, the phase-contrast effect may be added in cases where low-density media are employed. We obtained spatial resolutions of approximately 110  $\mu\text{m}$  using twofold magnification imaging using the II even when a 100- $\mu\text{m}$ -focus tube was employed. In order to observe fine blood vessels of less than 100  $\mu\text{m}$ , the spatial resolution of the radiography system should be improved to approximately 50  $\mu\text{m}$  using the II driven in a high-resolution mode, and the iodine density should be increased. At a tube voltage of 60 kV and a current of 0.50 mA, the photon number was approximately  $4 \times 10^7$  photons/( $\text{cm}^2 \cdot \text{s}$ ) at 1.0 m from the source, and photon count rate can be increased easily using a rotating anode microfocuse tube developed by Hitachi Medical Corporation. Because the focus diameter of the tube has been decreased to 10  $\mu\text{m}$ , a high-resolution real-time magnification radiography system will become possible.

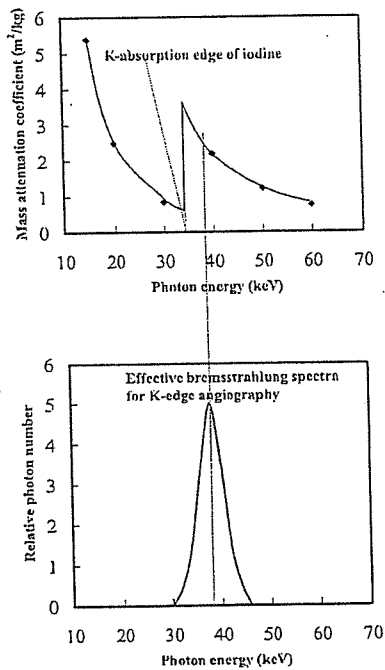


Fig. 8. Mass attenuation coefficients of iodine and effective bremsstrahlung x-rays for enhanced K-edge angiography.

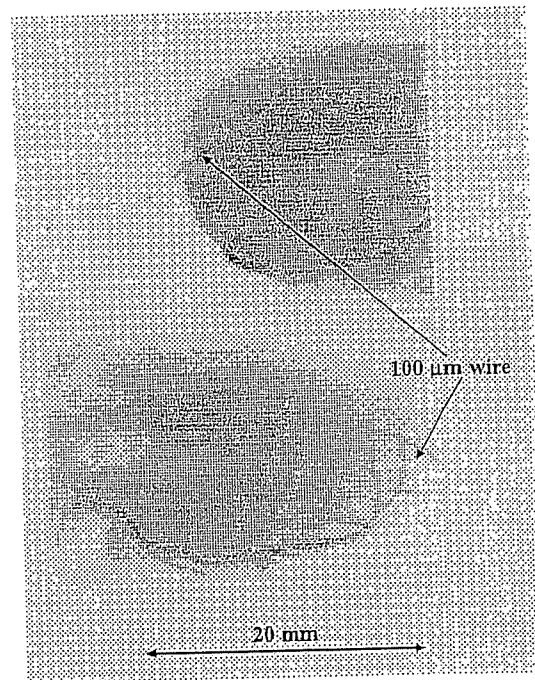


Fig. 9. Angiogram of an extracted rabbit heart using iodine microspheres.

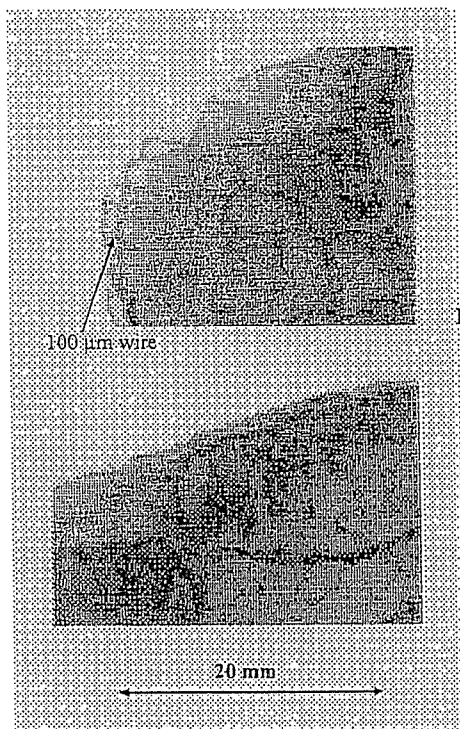


Fig. 10. Angiograms of an extracted dog heart.

#### ACKNOWLEDGMENT

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, and 16591222) and Advanced Medical Scientific Research from MECSS, Health and Labor Sciences Research Grants (RAMT-nano-001, RHGTEFB-genome-005 and RHGTEFB-saisei-003), and grants from the Keiryō Research Foundation, Promotion and Mutual Aid Corporation for Private Schools of Japan, Japan Science and Technology Agency (JST), and New Energy and Industrial Technology Development Organization (NEDO, Industrial Technology Research Grant Program in '03).

#### REFERENCES

1. E. Sato, S. Kimura, S. Kawasaki, H. Isobe, K. Takahashi, Y. Tamakawa and T. Yanagisawa, "Repetitive flash x-ray generator utilizing a simple diode with a new type of energy-selective function," *Rev. Sci. Instrum.*, **61**, 2343-2348, 1990.
2. A. Shikoda, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa, "Repetitive flash x-ray generator having a high-durability diode driven by a two-cable-type line pulser," *Rev. Sci. Instrum.*, **65**, 850-856, 1994.
3. E. Sato, K. Takahashi, M. Sagae, S. Kimura, T. Oizumi, Y. Hayasi, Y. Tamakawa and T. Yanagisawa, "Sub-kilohertz flash x-ray generator utilizing a glass-enclosed cold-cathode triode," *Med. & Biol. Eng. & Comput.*, **32**, 289-294, 1994.
4. K. Takahashi, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa, "Fundamental study on a long-duration flash x-ray generator with a surface-discharge triode," *Jpn. J. Appl. Phys.*, **33**, 4146-4151, 1994.
5. E. Sato, M. Sagae, E. Tanaka, Y. Hayasi, R. Germer, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube," *Jpn. J. Appl. Phys.*, **43**, 7324-7328, 2004.
6. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Compact monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube," *Med. Phys.*, **32**, 49-54, 2005.
7. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama and H. Ido,

- "Quasi-monochromatic flash x-ray generator utilizing weakly ionized linear copper plasma," *Rev. Sci. Instrum.*, **74**, 5236-5240, 2003.
8. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Sharp characteristic x-ray irradiation from weakly ionized linear plasma," *J. Electron Spectrosc. Related Phenom.*, **137-140**, 713-720, 2004.
9. E. Sato, E. Tanaka, H. Mori, T. Kawai, S. Sato and K. Takayama, "Clean monochromatic x-ray irradiation from weakly ionized linear copper plasma," *Opt. Eng.*, **44**, 049002-1-6, 2005.
10. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Inoue, A. Ogawa, S. Sato, K. Takayama, J. Onagawa, "X-ray spectra from weakly ionized linear copper plasma," *Jpn. J. Appl. Phys.*, **45**, 5301-5306, 2006.
11. T. J. Davis, D. Gao, T. E. Gureyev, A. W. Stevenson and S. W. Wilkins, "Phase-contrast imaging of weakly absorbing materials using hard x-rays," *Nature*, **373**, 595-597, 1995.
12. A. Momose, T. Takeda, Y. Itai and K. Hirano, "Phase-contrast x-ray computed tomography for observing biological soft tissues," *Nature Medicine*, **2**, 473-475, 1996.
13. H. Mori, K. Hyodo, E. Tanaka, M. U. Mohammed, A. Yamakawa, Y. Shinozaki, H. Nakazawa, Y. Tanaka, T. Sekka, Y. Iwata, S. Honda, K. Umetani, H. Ueki, T. Yokoyama, K. Tanioka, M. Kubota, H. Hosaka, N. Ishizawa and M. Ando, "Small-vessel radiography in situ with monochromatic synchrotron radiation," *Radiology*, **201**, 173-177, 1996.
14. K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita and J. Tada, "Development of a two-dimensional imaging system for clinical applications of intravenous coronary angiography using intense synchrotron radiation produced by a multipole wiggler," *J. Synchrotron Radiat.*, **5**, 1123-1126, 1998.
15. A. Ishisaka, H. Ohara and C. Honda, "A new method of analyzing edge effect in phase contrast imaging with incoherent x-rays," *Opt. Rev.*, **7**, 566-572, 2000.
16. E. Sato, K. Sato and Y. Tamakawa, "Film-less computed radiography system for high-speed imaging," *Ann. Rep. Iwate Med. Univ. Sch. Lib. Arts and Sci.*, **35**, 13-23, 2000.
17. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Demonstration of enhanced K-edge angiography using a cerium target x-ray generator," *Med. Phys.*, **31**, 3017-3021, 2004.
18. E. Sato, A. Yamadera, E. Tanaka, H. Mori, T. Kawai, F. Ito, T. Inoue, A. Ogawa, S. Sato, K. Takayama, J. Onagawa and H. Ido, "X-ray spectra from a cerium target and their application to cone beam K-edge angiography," *Opt. Eng.*, **44**, 096502-1-6, 2005.
19. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Inoue, A. Ogawa, A. Yamadera, S. Sato, F. Ito, K. Takayama, J. Onagawa and H. Ido, "Variations in cerium x-ray spectra and enhanced K-edge angiography," *Jpn. J. Appl. Phys.*, **44**, 8204-8209, 2005.
- \*dresato@iwate-med.ac.jp; phone +81-19-651-5111; fax +81-19-654-9282

# Super-characteristic x-ray generator utilizing a pipe and rod target

Eiichi Sato<sup>a\*</sup>, Etsuro Tanaka<sup>b</sup>, Hidezo Mori<sup>c</sup>, Toshiaki Kawai<sup>d</sup>, Takashi Inoue<sup>e</sup>, Akira Ogawa<sup>e</sup>, Mitsuru Izumisawa<sup>f</sup>, Kiyomi Takahashi<sup>g</sup>, Shigehiro Sato<sup>g</sup>, Toshio Ichimaru<sup>h</sup> and Kazuyoshi Takayama<sup>i</sup>

<sup>a</sup>Department of Physics, Iwate Medical University, 3-16-1 Honchodori, Morioka 020-0015, Japan

<sup>b</sup>Department of Nutritional Science, Faculty of Applied Bio-science, Tokyo University of Agriculture, 1-1-1 Sakuragaoka, Setagaya-ku, Tokyo 156-8502, Japan

<sup>c</sup>Department of Neurosurgery, School of Medicine, Iwate Medical University, 19-1 Uchimaru, Morioka 020-8505, Japan

<sup>d</sup>Electron Tube Division #2, Hamamatsu Photonics K.K., 314-5 Shimokanzo, Iwata 438-0193, Japan

<sup>e</sup>Department of Neurosurgery, School of Medicine, Iwate Medical University, 19-1 Uchimaru, Morioka 020-8505, Japan

<sup>f</sup>Department of Oral Radiology, School of Dentistry, Iwate Medical University, 1-3-27 Chuo, Morioka 020-0021, Japan

<sup>g</sup>Department of Microbiology, School of Medicine, Iwate Medical University, 19-1 Uchimaru, Morioka 020-8505, Japan

<sup>h</sup>Department of Radiological Technology, School of Health Sciences, Hirosaki University, 66-1 Honcho, Hirosaki 036-8564, Japan

<sup>i</sup>Tohoku University Biomedical Engineering Research Organization, Tohoku University, 2-1-1 Katahira, Sendai 980-8577, Japan

## ABSTRACT

This generator consists of the following components: a constant high-voltage power supply, a filament power supply, a turbomolecular pump, and an x-ray tube. The x-ray tube is a demountable diode which is connected to the turbomolecular pump and consists of the following major devices: a tungsten hairpin cathode (filament), a focusing (Wehnelt) electrode, a polyethylene terephthalate x-ray window 0.25 mm in thickness, a stainless-steel tube body, a pipe target, and a rod target. The pipe and rod targets are useful for forming linear and cone beams, respectively. In the x-ray tube, the positive high voltage is applied to the anode (target) electrode, and the cathode is connected to the tube body (ground potential). In this experiment, the tube voltage applied was from 12 to 20 kV, and the tube current was regulated to within 0.10 mA by the filament temperature. The exposure time is controlled in order to obtain optimum x-ray intensity. The electron beams from the cathode are converged to the target by the focusing electrode, and clean K-series characteristic x-rays are produced through the focusing electrode without using a filter. The x-ray intensities of the pipe and rod targets were 1.29 and 4.28  $\mu\text{Gy/s}$  at 1.0 m from the x-ray source with a tube voltage of 15 kV and a tube current of 0.10 mA, and quasi-monochromatic radiography was performed using a computed radiography system.

**Keywords:** demountable x-ray tube, electron-impact source, line beam, cone beam, quasi-monochromatic x-rays, K-series characteristic x-rays, Sommerfeld's theory

## 1. INTRODUCTION

Gas-discharge capillaries play significant roles in irradiation of soft x-ray lasers,<sup>1-3</sup> and the laser photon energy has been increasing. Subsequently, large-scale x-ray free electron laser sources<sup>4</sup> are constructing as a new-generation radiation source for producing monochromatic coherent x-rays to perform various research projects including biomedical applications. However, it is quite difficult to increase the maximum photon energy to 10 keV or beyond.

Hard X-Ray and Gamma-Ray Detector Physics and Penetrating Radiation Systems VIII,  
edited by Larry A. Franks, Arnold Burger, Ralph E. James, H. Bradford Barber, F. Patrick Doty, Hans Roehrig,  
Proc. of SPIE Vol. 6319, 6319Q, (2006) · 0277-786X/06/\$15 · doi: 10.1117/12.679243

Proc. of SPIE Vol. 6319 6319Q-1

To produce short x-ray pulses, several various flash x-ray generators utilizing high-voltage condensers have been developed, and high-speed radiography has been demonstrated. In particular, the importance of forming weakly ionized plasma source<sup>5-8</sup> is well reported to produce clean K-series characteristic x-rays, and the second and fourth harmonic x-rays of the fundamental K-series characteristic x-rays from copper and nickel targets have been confirmed. The x-ray intensities of the harmonics increase with increases in the charging voltage, and the harmonic bremsstrahlung rays survive due to the x-ray resonance in the plasma. However, it is not easy to produce high-photon-energy K-rays using linear plasmas, since the plasmas readily transmit high-photon-energy bremsstrahlung x-rays. In view of this situation, we have developed new flash x-ray generators<sup>9-11</sup> to produce high-photon-energy K-rays of molybdenum, cerium, tantalum, and tungsten.

At present, monochromatic parallel x-ray beams from synchrotrons utilizing silicon crystals are used in various fields including medical imaging. In particular, x-rays with photon energies ranging from 33.3 to 35 keV have been employed to perform enhanced K-edge angiography<sup>12,13</sup> because the rays are absorbed effectively by iodine-based contrast media with an iodine K-edge of 33.2 keV. This imaging plays significant roles in the diagnosis of coronary arteries, fine blood vessels in regenerative medicine, and capillaries in tumors. In contrast, small-scale steady-state monochromatic parallel and cone beams<sup>14-16</sup> can be employed to perform medical imaging in hospitals.

In this research, we developed an x-ray generator used to perform a preliminary experiment for generating clean K-series characteristic x-rays using a pipe and rod target by angle dependence of the bremsstrahlung x-rays.

## 2. GENERATOR

Figure 1 shows a block diagram of a compact characteristic (quasi-monochromatic) x-ray generator. This generator consists of the following components: a constant high-voltage power supply (SL150, Spellman), a DC filament power supply (SL150, Spellman), a turbomolecular pump, and an x-ray tube. The structures of the x-ray tube are illustrated in Figs. 2 and 3. The x-ray tube is a demountable diode which is connected to the turbomolecular pump with a pressure of approximately 0.5 mPa and consists of the following major devices: a tungsten hairpin cathode (filament), a focusing (Wehnelt) electrode, a polyethylene terephthalate x-ray window 0.25 mm in thickness, a stainless-steel tube body, a rod copper target of 3.0 mm in diameter, and a pipe copper target with an outside and a bore diameters of 5.0 and 4.0, respectively. In the x-ray tube, the positive high voltage is applied to the anode (target) electrode, and the cathode is connected to the tube body (ground potential). In this experiment, the tube voltage applied was from 12 to 20 kV, and the tube current was regulated to within 0.10 mA by the filament temperature. The exposure time is controlled in order to obtain optimum x-ray intensity. The electron beams from the cathode are converged to the target by the focusing electrode, and x-rays are produced through the focusing electrode. Because bremsstrahlung rays are not emitted in the opposite direction to that of electron trajectory in Sommerfeld's theory<sup>20</sup> (Figs. 4 and 5), clean molybdenum K-series x-rays can be produced without using a filter.

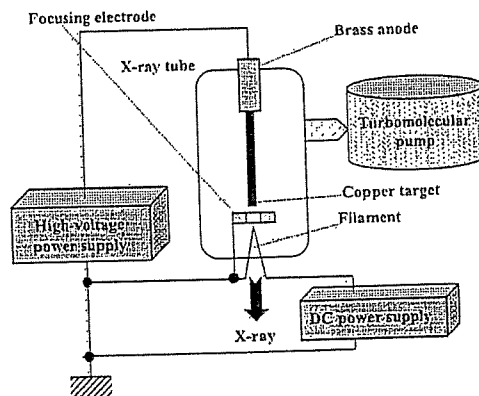


Fig. 1. Block diagram including the main transmission line of the compact x-ray generator with a quasi-monochromatic diode.

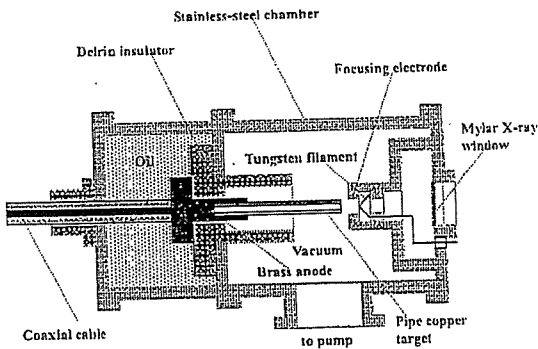


Fig. 2. Schematic drawing of the characteristic x-ray tube with a pipe copper target

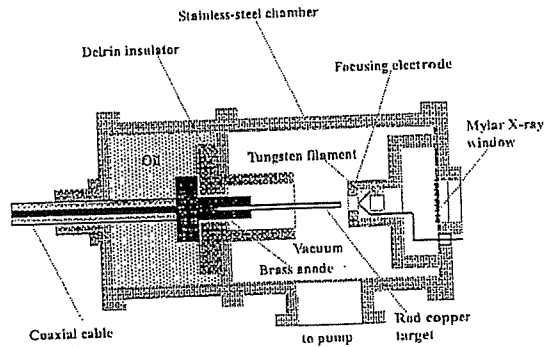


Fig. 3. Structure of the characteristic x-ray tube with a rod copper target.

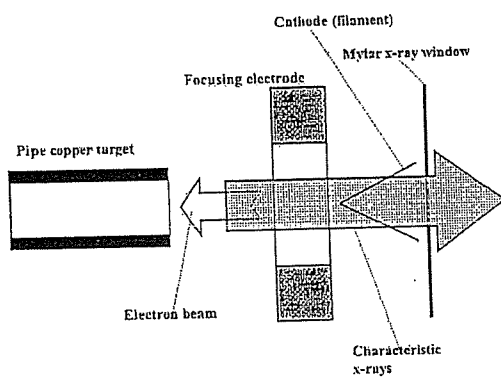


Fig. 4. K-photon irradiation from the pipe-target x-ray tube.

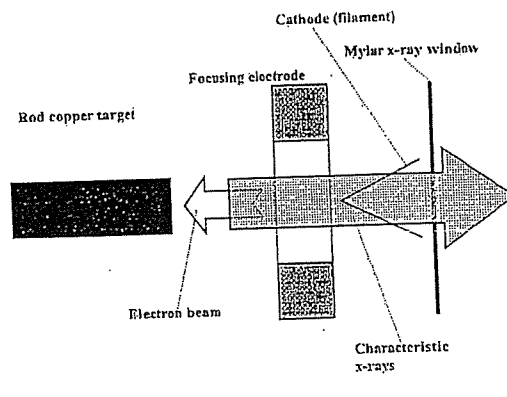


Fig. 5. K-photon irradiation from the rod-target x-ray tube.

### 3. CHARACTERISTICS

#### 3.1 X-ray intensity

X-ray intensities from the pipe and rod targets were measured by a Victoreen 660 ionization chamber at 1.0 m from the x-ray source (Figs. 6 and 7). At a constant tube current of 0.10 mA, the x-ray intensity increased when the tube voltage was increased. In this measurement, the intensities of the pipe and rod targets were 1.29 and 4.28  $\mu\text{Gy/s}$ , respectively, at 1.0 m from the source with a tube voltage of 15 kV.

#### 3.2 X-ray source

In order to measure images of the x-ray sources, we employed a pinhole camera with a hole diameter of 100  $\mu\text{m}$  in conjunction with a computed radiography (CR) system (Figs. 8 and 9). When the tube voltage was increased using the pipe target, the spot intensities increased, and the maximum diameter was equal to the bore diameter. On the other hand, both the intensity and diameter increased with increases in the tube voltage, and the maximum diameter was approximately 2.2 mm.

#### 3.3 X-ray spectra

X-ray spectra were measured using a silicon detector (XR-100CR, Amptek). We observed sharp K lines, and the characteristic x-ray intensities substantially increased with increases in the tube voltage (Figs. 10 and 12). Clean K lines were left by a 10- $\mu\text{m}$ -thick copper filter, and the  $K\alpha$  lines were selected out by absorbing  $K\beta$  lines using a 10- $\mu\text{m}$ -thick nickel filter (Figs. 11 and 13).

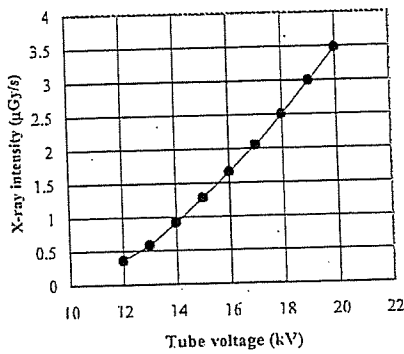


Fig. 6. X-ray intensity at 1.0 m from the pipe target according to changes in the tube voltage with a tube current of 0.10 mA.

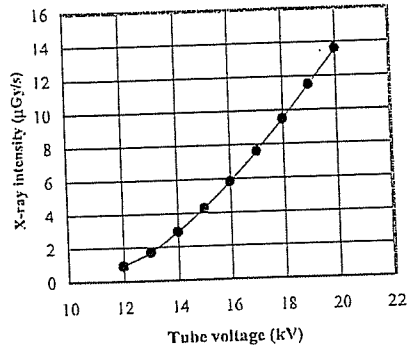


Fig. 7. X-ray intensity at 1.0 m from the rod target with changing the tube voltage with a tube current of 0.10 mA.

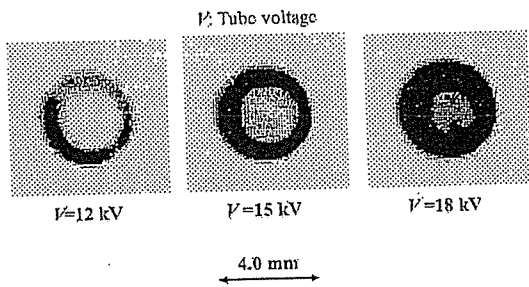


Fig. 8. Images of the characteristic x-ray source from the pipe target with changes in the tube voltage.

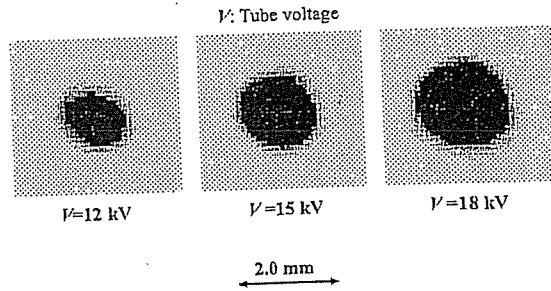


Fig. 9. Images of the characteristic x-ray source from the rod target.

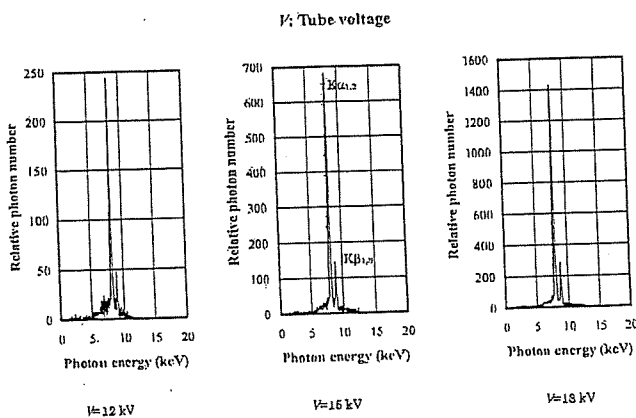


Fig. 10. X-ray spectra from the pipe target with changes in the tube voltage.

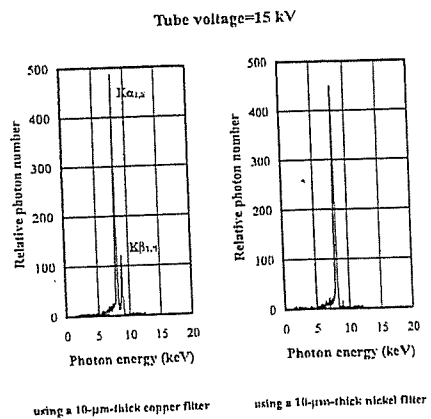


Fig. 11. X-ray spectra from the pipe target according to insertion of filters.

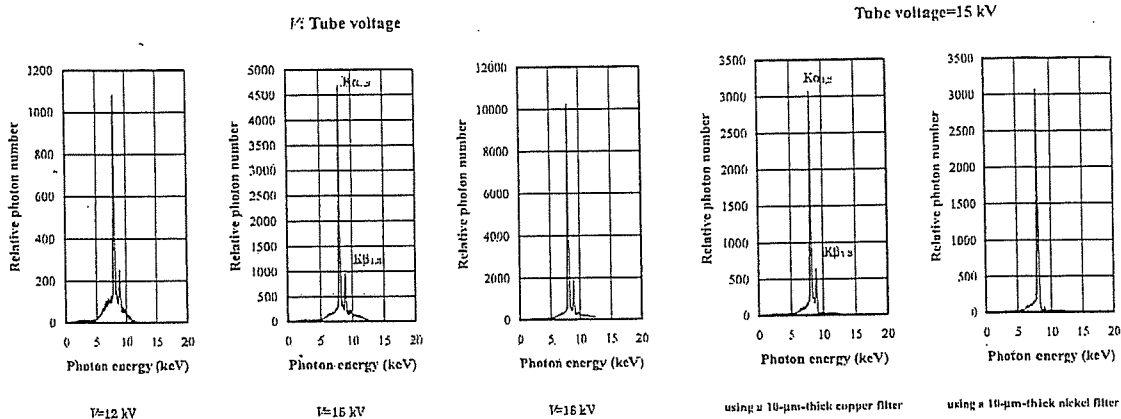


Fig. 12. X-ray spectra from the rod target with changing the tube voltage

Fig. 13. X-ray spectra from the rod target according to insertion of filters.

#### 4. CONCLUSIONS AND OUTLOOK

We developed a super-characteristic x-ray generator with the pipe and rod targets and succeeded in producing copper K lines. The characteristic x-ray intensity increased with increases in the tube voltage, and monochromatic  $K\alpha$  lines were left by the nickel filter.

In the spectrum measurements, we usually employ a silicon detector and a lithium fluoride curved crystal. The detector is useful for measuring the total spectra, including scattering beams. On the other hand, the spectra from only the x-ray source can be measured using the crystal by selecting Bragg's angle. Using the crystal in conjunction with a computed radiography system, we observed clean copper K lines.

In this preliminary experiment, although the maximum tube voltage and current were 20 kV and 0.10 mA, the voltage and current could be increased to 100 kV and 1.0 mA, respectively. Using the rod target, the generator produced maximum number of characteristic photons from the rod target was approximately  $1 \times 10^6$  photons/( $\text{cm}^2 \cdot \text{s}$ ) at 1.0 m from the source, and the photon count rate can be increased easily by increasing the current.

Currently, the copper K-series characteristic x-rays are useful for extremely soft radiography, and the photon energies of characteristic x-rays can be selected by the target element. In particular, the pipe target is useful for forming monochromatic line beams by decreasing the bore diameter.

#### ACKNOWLEDGMENT

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, and 16591222) and Advanced Medical Scientific Research from MECSST, Health and Labor Sciences Research Grants (RAMT-nano-001, RHGTEFB-genome-005 and RHGTEFB-saisei-003), and grants from the Keiryō Research Foundation, Promotion and Mutual Aid Corporation for Private Schools of Japan, Japan Science and Technology Agency (JST), and New Energy and Industrial Technology Development Organization (NEDO, Industrial Technology Research Grant Program in '03).

#### REFERENCES

1. J.J. Rocca, V. Shlyaptsev, F.G. Tomasel, O.D. Cortazar, D. Hartshorn and J.L.A. Chilla, "Demonstration of a discharge pumped table-top soft x-ray laser," *Phys. Rev. Lett.*, 73, 2192-2195, 1994.
2. J.J.G. Rocca, J.L.A. Chilla, S. Sakadzic, A. Rahman, J. Filevich, E. Jankowska, E.C. Hammarsten, B.M. Lüther, H.C. Kapteyn, M. Murnane and V.N. Shlyapsev, "Advances in capillary discharge soft x-ray laser research," *SPIE*, 4505, 1-6, 2001.



3. S. Le Pape, Ph. Zeitoun, J.J.G. Rocca, A. Carillon, P. Dhez, M. Francois, S. Hubert, M. Idir and D. Ros, "Characterisation of an x-ray laser beam," *SPIE*, 4505, 23-34, 2001.
4. C. Gerth, "Free-electron laser at the TESLA test facility at DESY: toward a tunable short-pulsed soft x-ray source," *SPIE*, 4505, 131-145, 2001.
5. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing weakly ionized linear copper plasma," *Rev. Sci. Instrum.*, 74, 5236-5240, 2003.
6. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Sharp characteristic x-ray irradiation from weakly ionized linear plasma," *J. Electron Spectrosc. Related Phenom.*, 137-140, 713-720, 2004.
7. E. Sato, E. Tanaka, H. Mori, T. Kawai, S. Sato and K. Takayama, "Clean monochromatic x-ray irradiation from weakly ionized linear copper plasma," *Opt. Eng.*, 44, 049002-1-6, 2005.
8. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Inoue, A. Ogawa, S. Sato, K. Takayama, J. Onagawa, "X-ray spectra from weakly ionized linear copper plasma," *Jpn. J. Appl. Phys.*, 45, 5301-5306, 2006.
9. E. Sato, M. Sagae, E. Tanaka, Y. Hayasi, R. Germer, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube," *Jpn. J. Appl. Phys.*, 43, 7324-7328, 2004.
10. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Compact monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube," *Med. Phys.*, 32, 49-54, 2005.
11. E. Sato, Y. Hayasi, K. Kimura, E. Tanaka, H. Mori, T. Kawai, T. Inoue, A. Ogawa, S. Sato, K. Takayama, J. Onagawa and H. Ido, "Enhanced K-edge angiography utilizing tantalum plasma x-ray generator in conjunction with gadolinium-based contrast media," *Jpn. J. Appl. Phys.*, 44, 8716-8721, 2005.
12. H. Mori, K. Hyodo, E. Tanaka, M. U. Mohammed, A. Yamakawa, Y. Shinozaki, H. Nakazawa, Y. Tanaka, T. Sekka, Y. Iwata, S. Honda, K. Umetani, H. Ueki, T. Yokoyama, K. Tanioka, M. Kubota, H. Hosaka, N. Ishizawa and M. Ando, "Small-vessel radiography in situ with monochromatic synchrotron radiation," *Radiology*, 201, 173-177, 1996.
13. K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita and J. Tada, "Development of a two-dimensional imaging system for clinical applications of intravenous coronary angiography using intense synchrotron radiation produced by a multipole wiggler," *J. Synchrotron Radiat.*, 5, 1123-1126, 1998.
14. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Demonstration of enhanced K-edge angiography using a cerium target x-ray generator," *Med. Phys.*, 31, 3017-3021, 2004.
15. E. Sato, A. Yamadera, E. Tanaka, H. Mori, T. Kawai, F. Ito, T. Inoue, A. Ogawa, S. Sato, K. Takayama, J. Onagawa and H. Ido, "X-ray spectra from a cerium target and their application to cone beam K-edge angiography," *Opt. Eng.*, 44, 096502-1-6, 2005.
16. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Inoue, A. Ogawa, A. Yamadera, S. Sato, F. Ito, K. Takayama, J. Onagawa and H. Ido, "Variations in cerium x-ray spectra and enhanced K-edge angiography," *Jpn. J. Appl. Phys.*, 44, 8204-8209, 2005.

\*dresato@iwate-med.ac.jp; phone +81-19-651-5111; fax +81-19-654-9282

## Characteristic X-ray Generator Utilizing Angle Dependence of Bremsstrahlung X-ray Distribution

Eiichi SATO, Etsuro TANAKA<sup>1</sup>, Hidezo MORI<sup>2</sup>, Toshiaki KAWAI<sup>3</sup>, Takashi INOUE<sup>4</sup>, Akira OGAWA<sup>4</sup>, Shigehiro SATO<sup>5</sup>, Kazuyoshi TAKAYAMA<sup>6</sup> and Jun ONAGAWA<sup>7</sup>

*Department of Physics, Iwate Medical University, 3-16-1 Honchodori, Morioka 020-0015, Japan*

<sup>1</sup>*Department of Nutritional Science, Faculty of Applied Bio-science, Tokyo University of Agriculture,*

*1-1-1 Sakuragaoka, Setagaya-ku, Tokyo 156-8502, Japan*

<sup>2</sup>*Department of Cardiac Physiology, National Cardiovascular Center Research Institute, 5-7-1 Fujishirodai, Suita, Osaka 565-8565, Japan*

<sup>3</sup>*Electron Tube Division #2, Hamamatsu Photonics K.K., 314-5 Shimokanzo, Iwata, Shizuoka 438-0193, Japan*

<sup>4</sup>*Department of Neurosurgery, School of Medicine, Iwate Medical University, 19-1 Uchimarui, Morioka 020-8505, Japan*

<sup>5</sup>*Department of Microbiology, School of Medicine, Iwate Medical University, 19-1 Uchimarui, Morioka 020-8505, Japan*

<sup>6</sup>*Shock Wave Research Center, Institute of Fluid Science, Tohoku University, 2-1-1 Katahira, Sendai 980-8577, Japan*

<sup>7</sup>*Department of Applied Physics and Informatics, Faculty of Engineering, Tohoku Gakuin University,*

*1-13-1 Chuo, Tagajo, Miyagi 985-8537, Japan*

(Received November 17, 2005; revised December 24, 2005; accepted December 31, 2005; published online April 7, 2006)

This generator consists of the following components: a constant high-voltage power supply, a filament power supply, a turbomolecular pump, and an X-ray tube. The X-ray tube is a demountable diode which is connected to the turbomolecular pump and consists of the following major devices: a molybdenum rod target, a tungsten hairpin cathode (filament), a focusing (Wehnelt) electrode, a polyethylene terephthalate X-ray window 0.25 mm in thickness, and a stainless-steel tube body. In the X-ray tube, the positive high voltage is applied to the anode (target) electrode, and the cathode is connected to the tube body (ground potential). In this experiment, the tube voltage applied was from 22 to 36 kV, and the tube current was regulated to within 100  $\mu$ A by the filament temperature. The exposure time is controlled in order to obtain optimum X-ray intensity. The electron beams from the cathode are converged to the target by the focusing electrode, and clean K-series characteristic X-rays are produced through the focusing electrode without using a filter. The X-ray intensity was 26.6  $\mu$ Gy/s at 1.0 m from the X-ray source with a tube voltage of 30 kV and a tube current of 100  $\mu$ A, and quasi-monochromatic radiography was performed using a computed radiography system. [DOI: 10.1143/JJAP.45.2845]

**KEYWORDS:** demountable X-ray tube, electron-impact source, quasi-monochromatic X-rays, K-series characteristic X-rays, Sommerfeld's theory

### 1. Introduction

A great deal of effort has been devoted to the research and development of X-ray lasers in past years, and several different generators have been developed. Using tera-watt pulse lasers as pumping sources, a transient collisional excitation method has been proposed.<sup>1)</sup> Subsequently, capillary discharge soft X-ray laser generators<sup>2-4)</sup> have been developed and demonstrated. However, it is difficult to produce high-photon-energy X-ray lasers with energies 10 keV or beyond.

Recently, we have developed several different flash X-ray generators<sup>5-9)</sup> corresponding to specific radiographic objectives, and the plasma X-ray source has been growing with increases in the electrostatic energy in the condenser. By forming weakly ionized linear plasma using rod targets, we confirmed irradiation of clean K-series characteristic X-rays such as hard X-ray lasers from the plasma axial direction using a table-top flash X-ray generator.<sup>10-13)</sup> This super fluorescence has been employed to perform cone-beam monochromatic radiography such as iodine K-edge and gadolinium K-edge angiographies. Furthermore, because higher harmonic hard X-rays have been produced from the copper plasma, we have to confirm the irradiations of higher harmonics with charges in the target element.

Without forming plasmas, demountable flash X-ray tubes can be employed to perform fundamental study on producing monochromatic X-rays,<sup>14)</sup> and have succeeded in producing clean K-series characteristic X-rays. However, monochromatic flash radiography has had difficulties in controlling X-ray duration, and in performing magnification

radiography including phase-contrast effect.

At present, brilliant monochromatic parallel X-ray beams from synchrotron radiation are used in various fields including medical imaging,<sup>15-17)</sup> and large-scale X-ray free electron laser sources<sup>18)</sup> are constructing as a new-generation radiation source for producing monochromatic coherent X-rays. In contrast, small-scale steady-state monochromatic parallel and cone beams can be employed to perform medical imaging including phase-contrast radiography and K-edge angiography<sup>19)</sup> in hospitals.

In this paper, we developed an X-ray generator used to perform a preliminary experiment for generating clean K-series characteristic X-rays by angle dependence of the bremsstrahlung X-rays.

### 2. Generator

Figure 1 shows a block diagram of a compact characteristic (quasi-monochromatic) X-ray generator. This generator consists of the following components: a constant high-voltage power supply (SL150, Spellman), a DC filament power supply, a turbomolecular pump, and an X-ray tube. The structure of the X-ray tube is illustrated in Fig. 2. The X-ray tube is a demountable diode which is connected to the turbomolecular pump with a pressure of approximately 0.5 mPa and consists of the following major devices: a molybdenum rod target of 3.0 mm in diameter, a tungsten hairpin cathode (filament), a focusing (Wehnelt) electrode, a polyethylene terephthalate X-ray window 0.25 mm in thickness, and a stainless-steel tube body. In the X-ray tube, the positive high voltage is applied to the anode (target) electrode, and the cathode is connected to the tube body

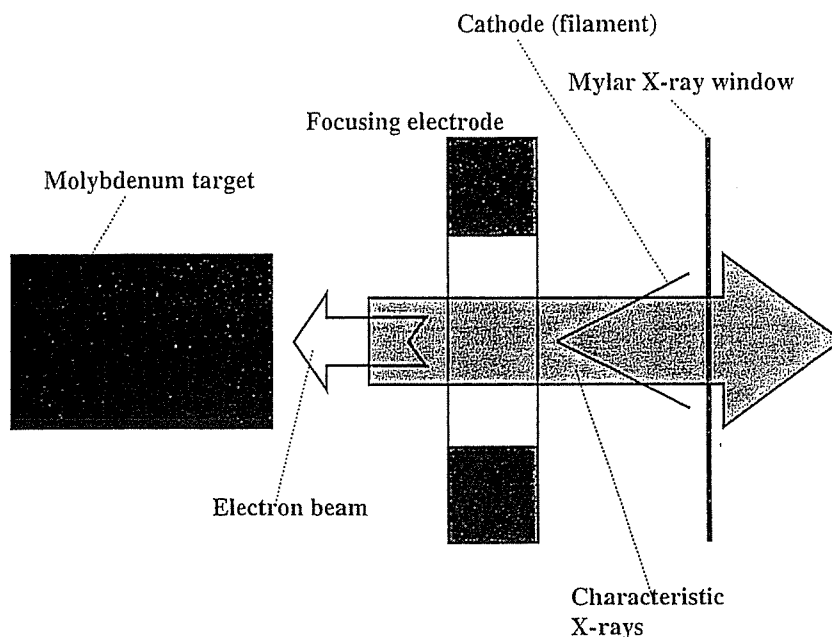


Fig. 3. K-photon irradiation from the X-ray tube.

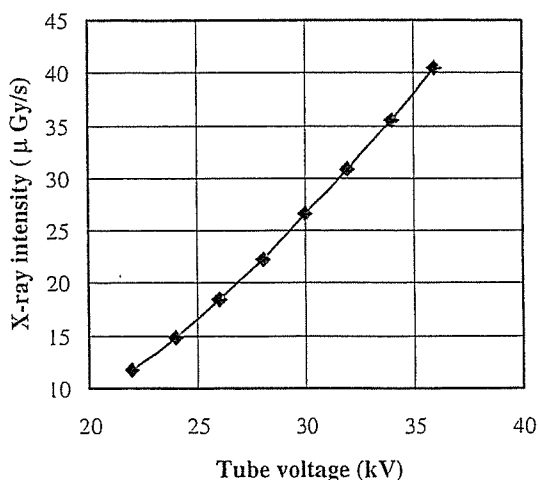


Fig. 4. X-ray intensity at 1.0m from the X-ray source according to changes in the tube voltage with a tube current of 100μA.

detected by an imaging plate of the CR system (Konica Minolta, Regius 150) with a wide dynamic range, and relative X-ray intensity was calculated from Dicom original digital data corresponding to X-ray intensity; the data was scanned by Dicom viewer in the film-less CR system. Subsequently, the relative X-ray intensity as a function of the data was calibrated using a conventional X-ray generator, and we confirmed that the intensity was proportional to the exposure time. Figure 6 shows measured spectra from the molybdenum target. We observed clean K lines, while bremsstrahlung rays were hardly detected. The characteristic X-ray intensity substantially increased with increases in the tube voltage.

#### 4. Radiography

The quasi-monochromatic radiography was performed by the CR system at 1.0 m from the X-ray source with the filter,

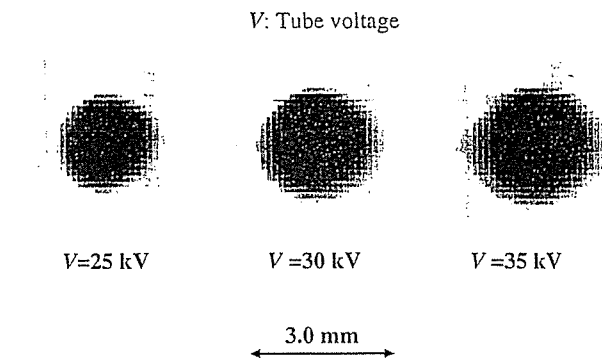


Fig. 5. Images of the characteristic X-ray source obtained using a pinhole camera with changes in the tube voltage.

and the tube voltage was 30 kV.

Firstly, rough measurements of image resolution were made using wires. Figure 7 shows radiograms of tungsten wires coiled around pipes made of poly(methyl methacrylate) (PMMA). Although the image contrast increased with increases in the wire diameter, a 50 μm-diameter wire could be observed.

A radiogram of a vertebra is shown in Fig. 8, and the fine structure of the vertebra was observed. Next, angiography was performed using iodine microspheres of 15 μm in diameter. Figures 9 and 10 show angiograms of a rabbit heart and thigh, respectively, and we could obtain high contrast images of coronary arteries and fine blood vessels.

#### 5. Conclusions and Outlook

In summary, we developed a new quasi-monochromatic X-ray generator with a molybdenum-target tube and succeeded in producing clean molybdenum K lines. The characteristic X-ray intensity increased with increases in the tube voltage, and monochromatic Kα rays were left by a zirconium filter.

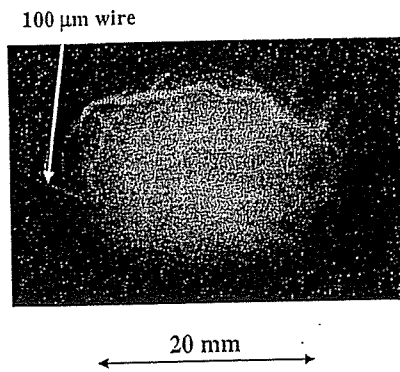


Fig. 9. Angiograms of a rabbit heart. Coronary arteries were visible.

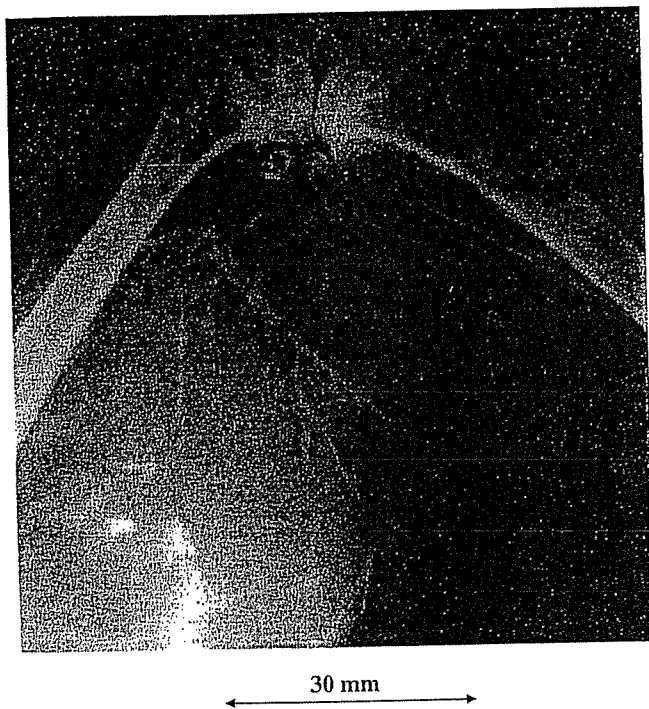


Fig. 10. Angiogram of a rabbit thigh. Fine blood vessels of approximately 100 μm were visible.

the target evaporation. Subsequently, the generator produced maximum number of characteristic photons was approximately  $1 \times 10^8$  photons/(cm<sup>2</sup>·s) at 1.0 m from the source, and the photon count rate can be increased easily by increasing the current.

In the present research, the molybdenum K-series characteristic X-rays are useful for mammography, and the photon energies of characteristic X-rays can be selected by the target element. In particular, enhanced K-edge angiography can be performed using a cerium target because cerium K $\alpha$  rays (34.6 keV) are absorbed easily by iodine-based contrast media with an iodine K-edge of 33.2 keV.

Using this angiography, coronary arteries and fine blood vessels formed in regenerative medicine may be observed with high contrasts. Furthermore, a flat panel detector is useful to observe blood flows for cases of cardiovascular disease.

#### Acknowledgment

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, and 16591222) and Advanced Medical Scientific Research from MECSS, Grants from Keiryō Research Foundation, The Promotion and Mutual Aid Corporation for Private School of Japan, JST (Test of Fostering Potential), NEDO, and MHLW (HLSRG, RAMT-nano-001, RHGTEFB-genome-005, and RGCD13C-1).

- 1) K. Nagashima, M. Tanaka, M. Nishikino, M. Kishimoto, M. Kado, T. Kawachi, N. Hasegawa, Y. Ochi, K. Sukegawa, R. Tai and K. Kato: Proc. SPIE 5197 (2003) 1.
- 2) J. J. Rocca, V. Shlyaptev, F. G. Tomasel, O. D. Cortazar, D. Hartshorn and J. L. A. Chilla: Phys. Rev. Lett. 73 (1994) 2192.
- 3) C. D. Macchietto, B. R. Benware and J. J. Rocca: Opt. Lett. 24 (1999) 1115.
- 4) J. J. G. Rocca, J. L. A. Chilla, S. Sakadzic, A. Rahman, J. Filevich, E. Jankowska, E. C. Hammarsten, B. M. Luther, H. C. Kapteyn, M. Murnane and V. N. Shlyapsev: Proc. SPIE 4505 (2001) 1.
- 5) E. Sato, S. Kimura, S. Kawasaki, H. Isobe, K. Takahashi, Y. Tamakawa and T. Yanagisawa: Rev. Sci. Instrum. 61 (1990) 2343.
- 6) K. Takahashi, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa: Jpn. J. Appl. Phys. 33 (1994) 4146.
- 7) E. Sato, K. Takahashi, M. Sagae, S. Kimura, T. Oizumi, Y. Hayasi, Y. Tamakawa and T. Yanagisawa: Med. Biol. Eng. Comput. 32 (1994) 289.
- 8) E. Sato, M. Sagae, K. Takahashi, A. Shikoda, T. Oizumi, Y. Hayasi, Y. Tamakawa and T. Yanagisawa: Med. Biol. Eng. Comput. 32 (1994) 295.
- 9) E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido: Med. Phys. 32 (2005) 49.
- 10) E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama and H. Ido: Rev. Sci. Instrum. 74 (2003) 5236.
- 11) E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido: J. Electron Spectrosc. Relat. Phenom. C 137-140 (2004) 713.
- 12) E. Sato, E. Tanaka, H. Mori, T. Kawai, S. Sato and K. Takayama: Opt. Eng. 44 (2005) 049002.
- 13) E. Sato, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, H. Ojima, K. Takayama and H. Ido: Proc. SPIE 5580 (2005) 146.
- 14) E. Sato, M. Sagae, E. Tanaka, Y. Hayasi, R. Germer, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido: Jpn. J. Appl. Phys. 43 (2004) 7324.
- 15) A. Momose, T. Takeda, Y. Itai and K. Hirano: Nat. Med. 2 (1996) 473.
- 16) H. Mori *et al.*: Radiology 201 (1996) 173.
- 17) K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita and J. Tada: J. Synchrotron Radiat. 5 (1998) 1123.
- 18) K. Lan, E. E. Fill and J. M. Vehn: Proc. SPIE 5197 (2003) 253.
- 19) E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido: Med. Phys. 31 (2004) 3017.
- 20) B. K. Agarwal: *X-ray Spectroscopy* (Springer-Verlag, New York, 1991) 2nd ed., p. 18.
- 21) E. Sato, K. Sato and Y. Tamakawa: Annu. Rep. Iwate Med. Univ. School Lib. Arts Sci. 35 (2000) 13.