

6. DISCUSSION AND CONCLUSIONS

In summary, we succeeded in producing K-series characteristic x rays of tantalum and in performing K-edge angiography using gadolinium contrast media with a K-edge of 50.2 keV, and this K-edge angiography could be a useful technique to decrease the dose absorbed by patients. Although we employed tantalum $K\alpha$ (57.1 keV) and $K\beta$ (approximately 65 keV) rays, $K\beta$ rays should be absorbed using an ytterbium oxide filter with an ytterbium K edge of 61.3 keV in order to increase the image contrast of blood vessels.

To perform K-edge angiography using gadolinium media, although an ytterbium target with a $K\alpha$ energy of 52.0 keV is useful, the ytterbium has a high reactivity. If we assume that the ytterbium is employed, an alloy target should be developed. In this research, we obtained sufficient x-ray intensity per pulse for angiography, and the intensity can be increased by increasing the electrostatic energies in the high-voltage condenser. At a condenser capacity of 150 nF, the generator produced instantaneous number of K photons was approximately 1×10^9 photons/cm² per pulse at 1.0 m from the source.

In the flash x-ray tube, bremsstrahlung x rays with energies higher than the K-edge are absorbed effectively by the weakly ionized plasma and are converted into fluorescent (characteristic) x rays. In conjunction with this property, because the bremsstrahlung x rays are not emitted in the opposite direction to that of electron acceleration, clean characteristic x rays are produced. Using this flash x-ray generator, with which the photon energy of characteristic x rays can be selected, quasi-monochromatic imaging such as enhanced K-edge angiography using iodine contrast media and mammography can be performed.

ACKNOWLEDGMENT

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, 16591181, and 16591222) and Advanced Medical Scientific Research from MECSS, Health and Labor Sciences Research Grants (RAMT-nano-001, RHGTEFB-genome-005 and RHGTEFB-saisei-003), Grants from Keiryō Research Foundation, The Promotion and Mutual Aid Corporation for Private Schools of Japan, Japan Science and Technology Agency (JST), and New Energy and Industrial Technology Development Organization (NEDO, Industrial Technology Research Grant Program in '03).

REFERENCES

1. T. J. Davis, D. Gao, T. E. Gureyev, A. W. Stevenson and S. W. Wilkins, "Phase-contrast imaging of weakly absorbing materials using hard x-rays," *Nature*, **373**, 595-597, 1995.
2. A. Momose, T. Takeda, Y. Itai and K. Hirano, "Phase-contrast x-ray computed tomography for observing biological soft tissues," *Nature Medicine*, **2**, 473-475, 1996.
3. M. Ando, A. Maksimenko, H. Sugiyama, W. Pattanasiriwisawa, K. Hyodo and C. Uyama, "A simple x-ray dark- and bright- field imaging using achromatic Laue optics," *Jpn. J. Appl. Phys.*, **41**, L1016-L1018, 2002.
4. A. C. Thompson, H. D. Zeman, G. S. Brown, J. Morrison, P. Reiser, V. Padmanabahn, L. Ong, S. Green, J. Giacomini, H. Gordon and E. Rubenstein, "First operation of the medical research facility at the NSLS for coronary angiography," *Rev. Sci. Instrum.*, **63**, 625-628, 1992.
5. H. Mori, K. Hyodo, E. Tanaka, M. U. Mohammed, A. Yamakawa, Y. Shinozaki, H. Nakazawa, Y. Tanaka, T. Sekka, Y. Iwata, S. Honda, K. Umetani, H. Ueki, T. Yokoyama, K. Tanioka, M. Kubota, H. Hosaka, N. Ishizawa and M. Ando, "Small-vessel radiography in situ with monochromatic synchrotron radiation," *Radiology*, **201**, 173-177, 1996.
6. K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita and J. Tada, "Development of a two-dimensional imaging system for clinical applications of intravenous coronary angiography using intense synchrotron radiation produced by a multipole wiggler," *J. Synchrotron Rad.*, **5**, 1123-1126, 1998.
7. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Demonstration of enhanced K-edge angiography using a cerium target x-ray generator," *Med. Phys.*, **31**, 3017-3021, 2004.
8. R. Germer, "X-ray flash techniques," *J. Phys. E: Sci. Instrum.*, **12**, 336-350, 1979.
9. E. Sato, S. Kimura, S. Kawasaki, H. Isobe, K. Takahashi, Y. Tamakawa and T. Yanagisawa, "Repetitive flash x-ray generator utilizing a simple diode with a new type of energy-selective function," *Rev. Sci. Instrum.*, **61**, 2343-2348, 1990.

10. A. Shikoda, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa, "Repetitive flash x-ray generator having a high-durability diode driven by a two-cable-type line pulser," *Rev. Sci. Instrum.*, **65**, 850-856, 1994.
11. E. Sato, K. Takahashi, M. Sagae, S. Kimura, T. Oizumi, Y. Hayasi, Y. Tamakawa and T. Yanagisawa, "Sub-kilohertz flash x-ray generator utilizing a glass-enclosed cold-cathode triode," *Med. & Biol. Eng. & Comput.*, **32**, 289-294, 1994.
12. K. Takahashi, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa, "Fundamental study on a long-duration flash x-ray generator with a surface-discharge triode," *Jpn. J. Appl. Phys.*, **33**, 4146-4151, 1994.
13. E. Sato, M. Sagae, K. Takahashi, A. Shikoda, T. Oizumi, Y. Hayasi, Y. Tamakawa and T. Yanagisawa, "10 kHz microsecond pulsed x-ray generator utilizing a hot-cathode triode with variable durations for biomedical radiography," *Med. & Biol. Eng. & Comput.*, **32**, 295-301, 1994.
14. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, H. Obara, T. Ichimaru, K. Takayama and H. Ido, "Irradiation of intense characteristic x-rays from weakly ionized linear molybdenum plasma," *Jpn. J. Med. Phys.*, **23**, 123-131, 2003.
15. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing weakly ionized linear copper plasma," *Rev. Sci. Instrum.*, **74**, 5236-5240, 2003.
16. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Sharp characteristic x-ray irradiation from weakly ionized linear plasma," *J. Electron Spectrosc. Related Phenom.*, **137-140**, 713-720, 2004.
17. E. Sato, M. Sagae, E. Tanaka, Y. Hayasi, R. Germer, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube," *Jpn. J. Appl. Phys.*, **43**, 7324-7328, 2004.
18. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Compact monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube," *Med. Phys.*, **32**, 49-54, 2005.
19. E. Sato, K. Sato and Y. Tamakawa, "Film-less computed radiography system for high-speed imaging," *Ann. Rep. Iwate Med. Univ. Sch. Lib. Arts and Sci.*, **35**, 13-23, 2000.

*dresato@iwate-med.ac.jp; phone +81-19-651-5111; fax +81-19-654-9282

Enhanced magnification angiography including phase-contrast effect using a 100- μm focus x-ray tube

Eiichi Sato^{*a}, Etsuro Tanaka^b, Hidezo Mori^c, Hiroki Kawakami^d, Toshiaki Kawai^d, Takashi Inoue^e, Akira Ogawa^e, Shigehiro Sato^f, Toshio Ichimaru^g, Kazuyoshi Takayama^h and Hideaki Idoⁱ

^a Department of Physics, Iwate Medical University, 3-16-1 Honchodori, Morioka 020-0015, Japan

^b Department of Nutritional Science, Faculty of Applied Bio-science, Tokyo University of Agriculture, 1-1-1 Sakuragaoka, Setagaya-ku 156-8502, Japan

^c Department of Cardiac Physiology, National Cardiovascular Center Research Institute, 5-7-1 Fujishirodai, Suita, Osaka 565-8565 Japan

^d Electron Tube Division #2, Hamamatsu Photonics K. K., 314-5 Shimokanzo, Iwata 438-0193, Japan

^e Department of Neurosurgery, School of Medicine, Iwate Medical University, 19-1 Uchimarui, Morioka 020-8505, Japan,

^f Department of Microbiology, School of Medicine, Iwate Medical University, 19-1 Uchimarui, Morioka 020-8505, Japan

^g Department of Radiological Technology, School of Health Sciences, Hirosaki University, 66-1 Honcho, Hirosaki 036-8564, Japan

^h Shock Wave Research Center, Institute of Fluid Science, Tohoku University, 2-1-1 Katahira, Sendai 980-8577, Japan

ⁱ Department of Applied Physics and Informatics, Faculty of Engineering, Tohoku Gakuin University, 1-13-1 Chuo, Tagajo 985-8537, Japan

ABSTRACT

A microfocus x-ray tube is useful in order to perform magnification digital radiography including phase-contrast effect. The 100- μm -focus x-ray generator consists of a main controller for regulating the tube voltage and current and a tube unit with a high-voltage circuit and a fixed anode x-ray tube. The maximum tube voltage, current, and electric power were 105 kV, 0.5 mA, and 50 W, respectively. Using a 3-mm-thick aluminum filter, the x-ray intensity was 26.0 $\mu\text{Gy/s}$ at 1.0 m from the source with a tube voltage of 60 kV and a current of 0.50 mA. Because the peak photon energy was approximately 38 keV using the filter with a tube voltage of 60 kV, the bremsstrahlung x-rays were absorbed effectively by iodine-based contrast media with an iodine K-edge of 33.2 keV. Magnification angiography including phase-contrast effect was performed by three-time magnification imaging with a computed radiography system using iodine-based microspheres 15 μm in diameter. In angiography of non-living animals, we observed fine blood vessels of approximately 100 μm with high contrasts.

Keywords: high-contrast angiography, magnification digital radiography, microfocus x-ray tube, energy-selective imaging, phase-contrast effect

1. INTRODUCTION

Conventional flash x-ray generators utilizing condensers are useful in order to perform high-speed radiography including biomedical applications, and several different generators have been developed.¹⁻⁷ In particular, plasma flash x-ray generators⁸⁻¹⁰ have been employed to produce clean K-series characteristic x-rays, and we have confirmed the irradiation of higher harmonic hard x-rays of $K\alpha$ and $K\beta$ lines. Without forming plasmas, demountable flash x-ray tubes can be employed to perform fundamental study on producing monochromatic x-rays,^{11,12} and have succeeded in producing clean characteristic x-rays using angle dependence of bremsstrahlung x-ray distribution in Sommerfeld's theory. However, monochromatic flash radiography has had difficulties in increasing x-ray duration, and in performing magnification

radiography including phase-contrast effect.

Synchrotrons are capable of producing high-dose-rate monochromatic parallel x-ray beams using a monochrocollimator, and the beams have been applied to phase-contrast radiography^{13,14} and enhanced K-edge angiography.^{15,16} In angiography, monochromatic x-rays with photon energies approximately 35 keV have been employed because the rays are absorbed effectively by iodine-based contrast media with an iodine K edge of 33.2 keV.

Without using synchrotrons, phase-contrast radiography for edge enhancement can be performed using a microfocus x-ray tube, and the enhancement have been applied in mammography achieved with a computed radiography (CR) system¹⁷ using a 100- μm -focus molybdenum tube.¹⁸ Subsequently, we have developed a cerium x-ray generator^{19,20} to perform enhanced K-edge angiography using cone beams, and have succeeded in observing fine blood vessels and coronary arteries with high contrasts using cerium K α rays of 34.6 keV. However, it is difficult to design the small focus cerium tube for angiography.

The magnification radiography is useful in order to improve the spatial resolution in digital radiography, and the phase contrast may come into effect in edge enhancement of comparatively large objects including thick blood vessels filled with low-density contrast media. Therefore, narrow photon energy bremsstrahlung x-rays with a peak energy of approximately 35 keV from a microfocus tungsten tube are useful to perform high-contrast high-resolution angiography. In the present research, we employed a 100- μm -focus tungsten tube, and performed enhanced magnification angiography including phase-contrast effect by controlling bremsstrahlung x-ray spectra using an aluminum filter.

2. PRINCIPLE OF ENHANCED ANGIOGRAPHY

Figure 1 shows the mass attenuation coefficients of iodine at the selected energies; the coefficient curve is discontinuous at the iodine K-edge. The effective bremsstrahlung x-ray spectra for K-edge angiography are shown above the iodine K-edge. Because iodine contrast media with a K-absorption edge of 33.2 keV absorb the rays easily, blood vessels were observed with high contrasts.

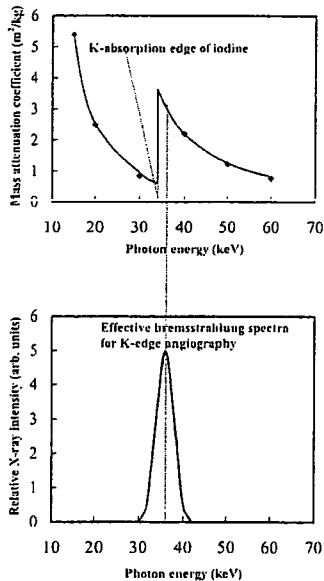


Figure 1: Mass attenuation coefficients of iodine and effective bremsstrahlung x-rays for enhanced K-edge angiography.

3. EXPERIMENTAL SETUP

Figure 2 shows the block diagram of a microfocus x-ray generator used in this experiment, and the generator consists of a main controller, an x-ray tube unit with a Cockcroft-Walton circuit, an insulation transformer, and a 100- μm -focus x-ray tube. The tube voltage, the current, and the exposure time can be controlled by the controller. The main circuit for producing x-rays is illustrated in Fig. 3, and employed the Cockcroft-Walton circuit in order to decrease the dimensions of the tube unit. In the x-ray tube, the positive and negative high voltages are applied to the anode and cathode electrodes,

respectively. The filament heating current is supplied by an AC power supply in the controller in conjunction with an insulation transformer which is used for isolation from the high voltage from the Cockcroft-Walton circuit. In this experiment, the tube voltage applied was from 45 to 70 kV, and the tube current was regulated to within 0.50 mA (maximum current) by the filament temperature. The exposure time is controlled in order to obtain optimum x-ray intensity, and narrow-photon-energy bremsstrahlung x-rays are produced using a 3.0-mm-thick aluminum filter for absorbing soft x-rays.

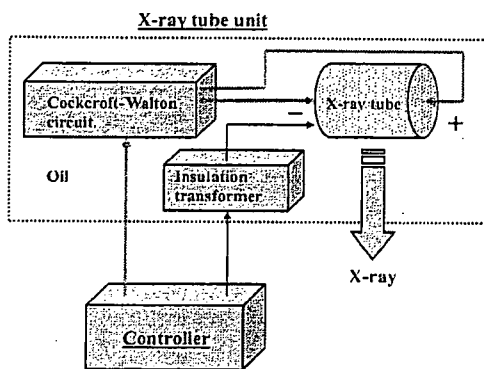


Figure 2: Block diagram of the x-ray generator.

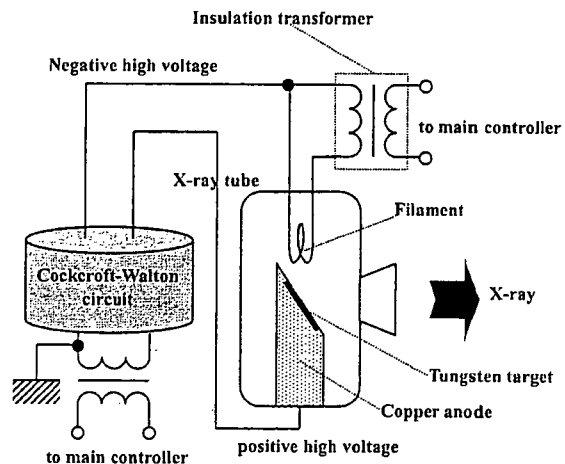


Figure 3: Electric circuit of the x-ray generator.

4 RESULTS

4.1 X-ray intensity

The x-ray intensity was measured by a Victoreen 660 ionization chamber at 1.0 m from the x-ray source using the filter (Fig. 4). At a constant tube current of 0.50 mA, the x-ray intensity increased when the tube voltage was increased. At a tube voltage of 60 kV, the intensity with the filter was 26.0 $\mu\text{Gy/s}$.

4.2 X-ray spectra

In order to measure x-ray spectra, we employed a cadmium telluride detector (CDTE2020X, Hamamatsu Photonics K. K.) with a photon energy resolution of approximately 1.7 keV (Fig. 5). When the tube voltage was increased, the bremsstrahlung x-ray intensity increased, and both the maximum photon energy and the spectrum peak energy increased. In order to perform K-edge angiography, bremsstrahlung x-rays of approximately 35 keV are useful, and the high-energy bremsstrahlung x-rays decrease the image contrast. Using this filter, because bremsstrahlung x-rays with energies higher than 60 keV were not absorbed easily, the tube voltage for angiography was determined as 60 kV.

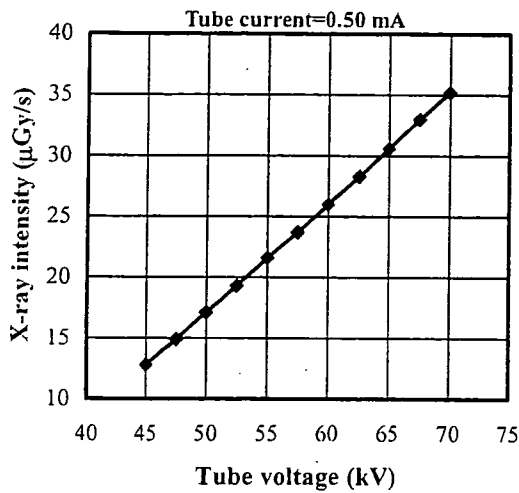


Figure 4: X-ray intensity ($\mu\text{Gy/s}$) as a function of tube voltage (kV) with a tube current of 0.50 mA.

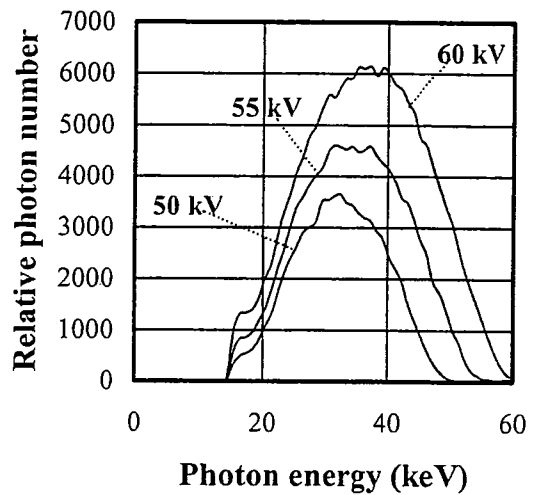


Figure 5. Bremsstrahlung x-ray spectra measured using a cadmium telluride detector with changes in the tube voltage.

4.3 Magnification radiography

The magnification radiography was performed by three-time magnification imaging using the CR system and the filter at a tube voltage of 60 kV, and the distance (between the x-ray source and the imaging plate) was 1.5 m (Fig. 6). Firstly, the spatial resolutions of conventional (cohesion) and magnification radiographies were made using a lead test chart. In the magnification radiography, 50 μm lines (10 line pairs) were clearly visible (Fig. 7). Subsequently, Fig. 8 shows radiograms of tungsten wires coiled around rods made of polymethyl methacrylate (PMMA). Although the image contrast decreased somewhat with decreases in the wire diameter, due to blurring of the image caused by the sampling pitch of 87.5 μm , a 50- μm -diameter wire could be observed. Radiograms of one set of a bolt and a nut are shown in Fig. 9, the edge of a bubble in the bolt and the seam between the bolt and the nut are visible in magnification radiography.

4.4 Enhanced magnification angiography

The magnification angiography was performed at the same conditions using iodine microspheres of 15 μm in diameter, and the microspheres (containing 37% iodine by weight) are very useful for making phantoms of non-living animals used for angiography. Angiogram of a rabbit heart is shown in Fig. 10, and the coronary arteries are visible. Figure 11 shows angiograms of a larger dog heart using iodine spheres. Although the image contrast decreased slightly with increases in the thickness of the PMMA plate facing the x-ray source, the coronary arteries of approximately 100 μm were observed using a 100-mm-thick plate.

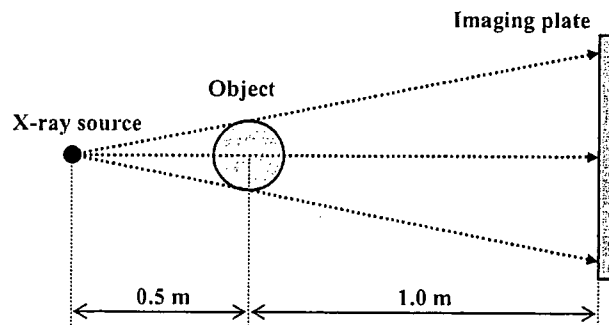


Figure 6. Three-time magnification imaging using an imaging plate in conjunction with a microfocus tube.

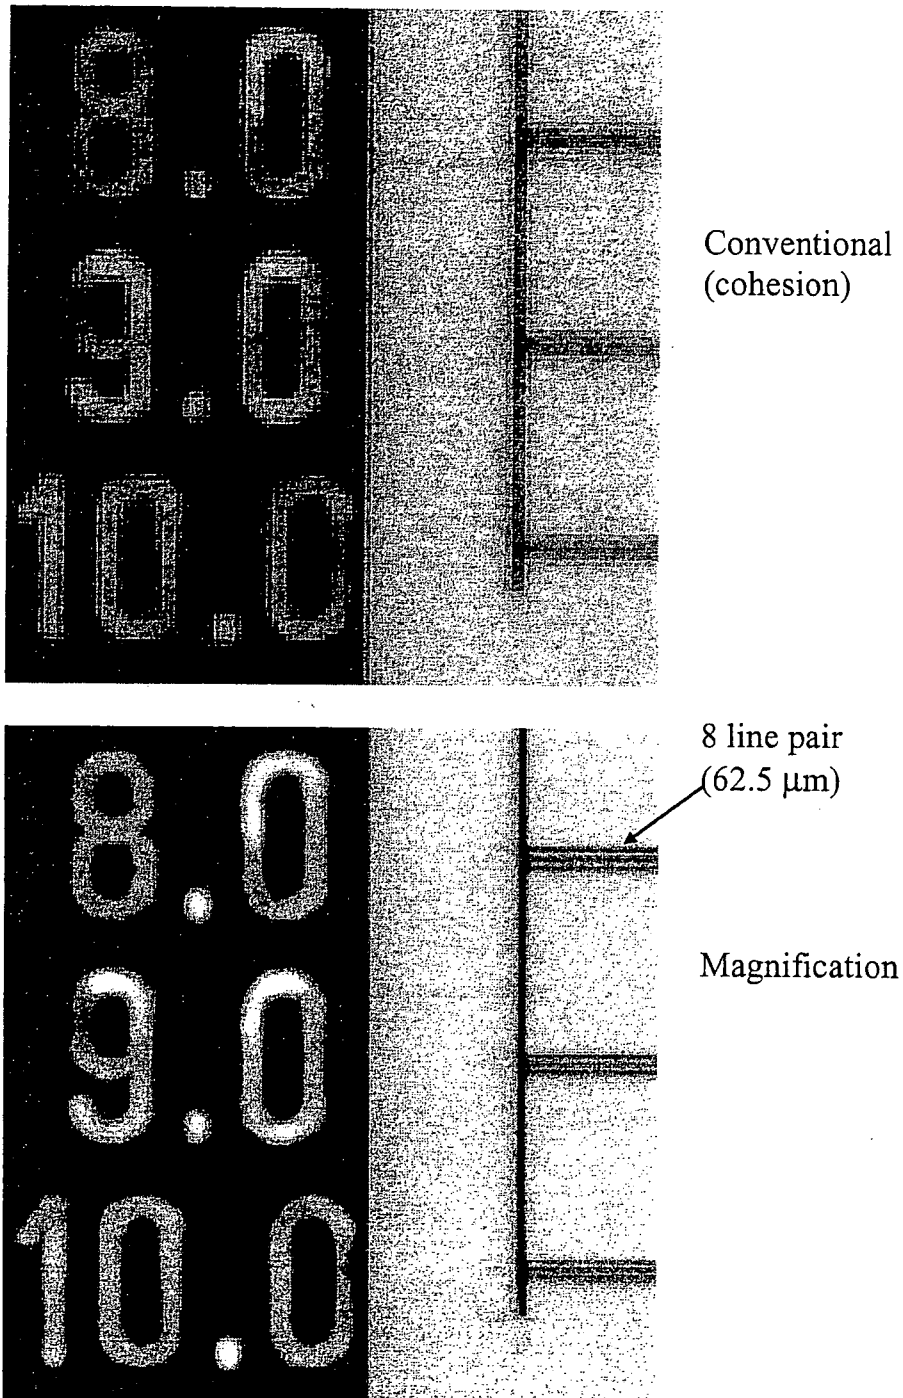


Figure 7. Radiogram of a test chart for measuring the spatial resolution.

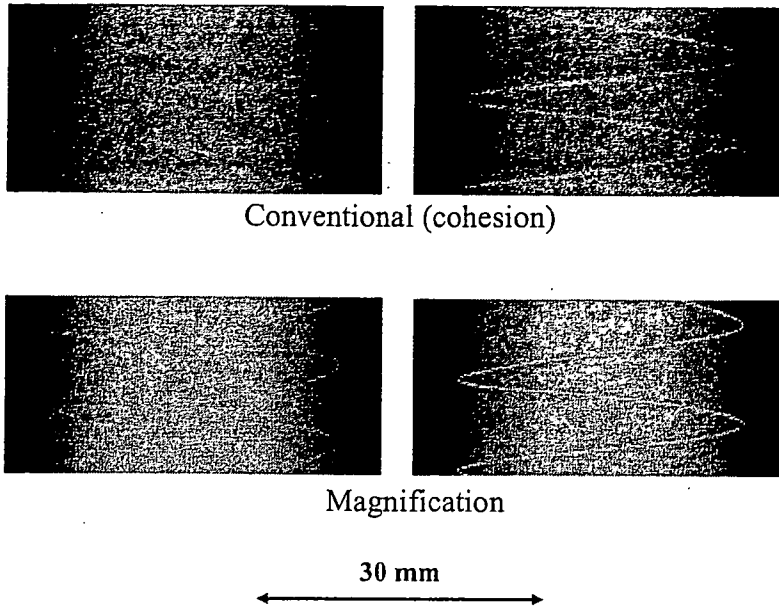


Figure 8. Radiograms of tungsten wires coiled around PMMA rods.

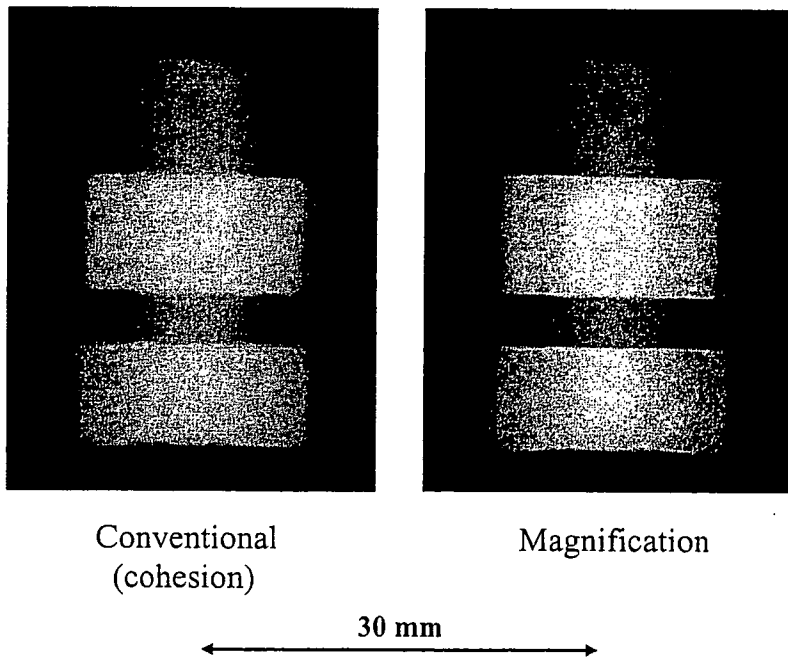


Figure 9. Radiograms of a set of a plastic bolt and a nut.

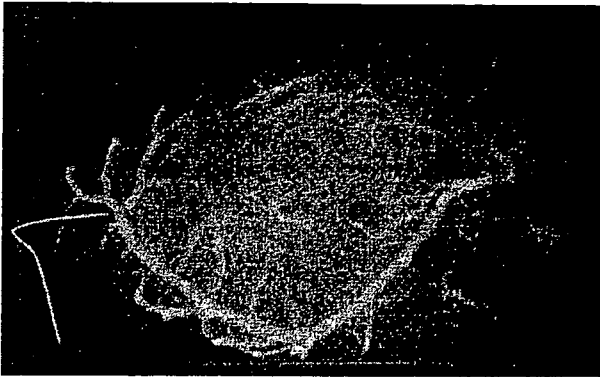



Figure 10: Angiogram of an extracted rabbit heart using iodine microspheres.

Magnification

20 mm



100 μ m wire

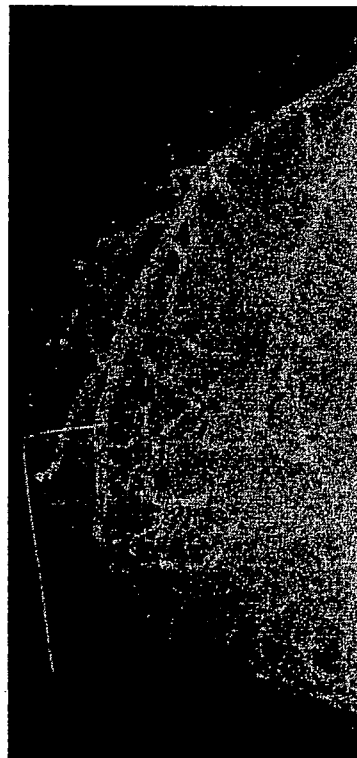

Using a 100-mm-thick
PMMA plate

20 mm




Figure 11. Angiograms of an extracted dog heart.

5. CONCLUSIONS AND OUTLOOK

In summary, we employed an x-ray generator with a 100- μm -focus tungsten tube and performed enhanced magnification angiography including phase-contrast effect using narrow-photon-energy bremsstrahlung x-rays with a peak photon energy of approximately 38 keV, which can be absorbed easily by iodine-based contrast media. The bremsstrahlung x-ray intensity substantially increased with increases in the tube voltage, and the tube voltage was determined as 60 kV in order to increase the image contrast. In enhanced angiography, although we obtained almost absorption-contrast images, phase-contrast effect may be added in cases where low-density media are employed.

Because the sampling pitch of the CR system is 87.5 μm , we obtained spatial resolutions of approximately 50 μm using 3-time magnification imaging even when a 100- μm -focus tube was employed. In order to observe fine blood vessels of less than 100 μm , the spatial resolution of the CR system should be improved to 43.8 μm (Konica Minolta Regius 190), and the iodine density should be increased.

At a tube voltage of 60 kV and a current of 0.50 mA, the maximum number of photons was approximately 4×10^7 photons/cm²·s at 1.0 m from the source, and the photon count rate can be increased easily using a rotating anode microfocus tube developed by Hitachi Medical Corporation. Recently, the maximum electric power of the microfocus x-ray tube has been increasing, and the kilowatt-range tube can be realized. Therefore, the dynamic magnification radiography is possible using a flat panel detector with a pixel size of less than 100 μm .

ACKNOWLEDGMENTS

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, 16591181, and 16591222) and Advanced Medical Scientific Research from MECSS, Health and Labor Sciences Research Grants (RAMT-nano-001, RHGTEFB-genome-005 and RHGTEFB-saisei-003), Grants from the Keiryō Research Foundation, The Promotion and Mutual Aid Corporation for Private Schools of Japan, Japan Science and Technology Agency (JST), and the New Energy and Industrial Technology Development Organization (NEDO, Industrial Technology Research Grant Program in '03).

REFERENCES

1. R. Germer, "X-ray flash techniques," *J. Phys. E: Sci. Instrum.*, **12**, 336-350, 1979.
2. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Portable x-ray generator utilizing a cerium-target radiation tube for angiography," *J. Electron Spectrosc. Related Phenom.*, **137-140**, 699-704, 2004.
3. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Demonstration of enhanced K-edge angiography using a cerium target x-ray generator," *Med. Phys.*, **31**, 3017-3021, 2004.
4. E. Sato, S. Kimura, S. Kawasaki, H. Isobe, K. Takahashi, Y. Tamakawa and T. Yanagisawa, "Repetitive flash x-ray generator utilizing a simple diode with a new type of energy-selective function," *Rev. Sci. Instrum.*, **61**, 2343-2348, 1990.
5. A. Shikoda, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa, "Repetitive flash x-ray generator having a high-durability diode driven by a two-cable-type line pulser," *Rev. Sci. Instrum.*, **65**, 850-856, 1994.
6. E. Sato, K. Takahashi, M. Sagae, S. Kimura, T. Oizumi, Y. Hayasi, Y. Tamakawa and T. Yanagisawa, "Sub-kilohertz flash x-ray generator utilizing a glass-enclosed cold-cathode triode," *Med. & Biol. Eng. & Comput.*, **32**, 289-294, 1994.
7. K. Takahashi, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa, "Fundamental study on a long-duration flash x-ray generator with a surface-discharge triode," *Jpn. J. Appl. Phys.*, **33**, 4146-4151, 1994.
8. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing weakly ionized linear copper plasma," *Rev. Sci. Instrum.*, **74**, 5236-5240, 2003.
9. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Sharp characteristic x-ray irradiation from weakly ionized linear plasma," *J. Electron Spectrosc. Related Phenom.*, **137-140**, 713-720, 2004.
10. E. Sato, E. Tanaka, H. Mori, T. Kawai, S. Sato and K. Takayama, "Clean monochromatic x-ray irradiation from weakly ionized linear copper plasma," *Opt. Eng.*, **44**, 049002-1-6, 2005.
11. E. Sato, M. Sagae, E. Tanaka, Y. Hayasi, R. Germer, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido: Quasi-monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube, *Jpn. J. Appl. Phys.*, **43**, 7324-7328, 2004.

12. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Compact monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube," *Med. Phys.*, **32**, 49-54, 2005.
 13. A. Momose, T. Takeda, Y. Itai and K. Hirano, "Phase-contrast x-ray computed tomography for observing biological soft tissues," *Nature Medicine*, **2**, 473-475, 1996.
 14. M. Ando, A. Maksimenko, H. Sugiyama, W. Pattanasiriwisawa, K. Hyodo and C. Uyama, "A simple x-ray dark- and bright- field imaging using achromatic Laue optics," *Jpn. J. Appl. Phys.*, **41**, L1016-L1018, 2002.
 15. H. Mori, K. Hyodo, E. Tanaka, M. U. Mohammed, A. Yamakawa, Y. Shinozaki, H. Nakazawa, Y. Tanaka, T. Sekka, Y. Iwata, S. Honda, K. Umetani, H. Ueki, T. Yokoyama, K. Tanioka, M. Kubota, H. Hosaka, N. Ishizawa and M. Ando, "Small-vessel radiography in situ with monochromatic synchrotron radiation," *Radiology*, **201**, 173-177, 1996.
 16. K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita and J. Tada, "Development of a two-dimensional imaging system for clinical applications of intravenous coronary angiography using intense synchrotron radiation produced by a multipole wiggler," *J. Synchrotron Rad.*, **5**, 1123-1126, 1998.
 17. E. Sato, K. Sato, T. Usuki and Y. Tamakawa, "Film-less computed radiography system for high-speed imaging," *Ann. Rep. Iwate Med. Univ. Sch. Lib. Arts and Sci.*, **35**, 13-23, 2000.
 18. A. Ishisaka, H. Ohara and C. Honda, "A new method of analyzing edge effect in phase contrast imaging with incoherent x-rays," *Opt. Rev.*, **7**, 566-572, 2000.
 19. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Portable x-ray generator utilizing a cerium-target radiation-tube for angiography," *J. Electron Spectrosc. Related Phenom.*, **137-140**, 699-704, 2004.
 20. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Demonstration of enhanced K-edge angiography using a cerium target x-ray generator," *Med. Phys.*, **31**, 3017-3021, 2004.
- *dresato@iwate-med.ac.jp; phone +81-19-651-5111; fax +81-19-654-9282

Monochromatic x-ray generator utilizing angle dependence of bremsstrahlung x-ray distribution

Eiichi Sato^{*a}, Etsuro Tanaka^b, Hidezo Mori^c, Toshiaki Kawai^d, Takashi Inoue^e, Akira Ogawa^c, Toshio Ichimaru^f, Kazuyoshi Takayama^g and Hideaki Ido^h

^a Department of Physics, Iwate Medical University, 3-16-1 Honchodori, Morioka 020-0015, Japan

^b Department of Nutritional Science, Faculty of Applied Bio-science, Tokyo University of Agriculture, 1-1-1 Sakuragaoka, Setagaya-ku 156-8502, Japan

^c Department of Cardiac Physiology, National Cardiovascular Center Research Institute, 5-7-1 Fujishirodai, Suita, Osaka 565-8565 Japan

^d Electron Tube Division #2, Hamamatsu Photonics K. K., 314-5 Shimokanzo, Iwata 438-0193, Japan

^e Department of Neurosurgery, School of Medicine, Iwate Medical University, 19-1 Uchimaru, Morioka 020-8505, Japan

^f Department of Radiological Technology, School of Health Sciences, Hirosaki University, 66-1 Honcho, Hirosaki 036-8564, Japan

^g Shock Wave Research Center, Institute of Fluid Science, Tohoku University, 2-1-1 Katahira, Sendai 980-8577, Japan

^h Department of Applied Physics and Informatics, Faculty of Engineering, Tohoku Gakuin University, 1-13-1 Chuo, Tagajo 985-8537, Japan

ABSTRACT

This generator consists of the following components: a constant high-voltage power supply, a filament power supply, a turbomolecular pump, and an x-ray tube. The x-ray tube is a demountable diode which is connected to the turbomolecular pump and consists of the following major devices: a molybdenum rod target, a tungsten hairpin cathode (filament), a focusing (Wehnelt) electrode, a polyethylene terephthalate x-ray window 0.25 mm in thickness, and a stainless-steel tube body. In the x-ray tube, the positive high voltage is applied to the anode (target) electrode, and the cathode is connected to the tube body (ground potential). In this experiment, the tube voltage applied was from 22 to 36 kV, and the tube current was regulated to within 100 μ A by the filament temperature. The exposure time is controlled in order to obtain optimum x-ray intensity. The electron beams from the cathode are converged to the target by the focusing electrode, and clean K α rays are produced through the focusing electrode using a 20- μ m-thick zirconium filter. The x-ray intensity was 12.1 μ Gy/s at 1.0 m from the x-ray source with a tube voltage of 30 kV and a tube current of 100 μ A, and monochromatic radiography was performed using a computed radiography system.

Keywords: demountable x-ray tube, electron-impact source, monochromatic x-rays, K α rays, Sommerfeld's theory

1. INTRODUCTION

Recently, we have developed several different flash x-ray generators¹⁻⁶ corresponding to specific radiographic objectives, and the plasma x-ray source has been growing with increases in the electrostatic energy in the condenser. By forming weakly ionized linear plasma⁷⁻¹⁰ using rod targets, we confirmed irradiation of clean K-series characteristic x-rays such as hard x-ray lasers from the plasma axial direction using a table-top flash x-ray generator. This super fluorescence has been employed to perform cone-beam monochromatic radiography such as iodine K-edge angiography.¹¹ Furthermore, because higher harmonic hard x-rays have been produced from the copper plasma, we have to confirm the irradiations of higher harmonics with charges in the target element.

At present, brilliant monochromatic parallel x-ray beams from synchrotron radiation are used in various fields including medical imaging,¹²⁻¹⁵ and large-scale x-ray free electron laser sources are constructing as a new-generation radiation

source for producing monochromatic coherent x-rays. In contrast, small-scale steady-state monochromatic parallel and cone beams can be employed to perform medical imaging including phase-contrast radiography and K-edge angiography^{16,17} in hospitals.

In this paper, we developed a monochromatic x-ray generator, used to perform a preliminary experiment for generating clean molybdenum $K\alpha$ rays by angle dependence of the bremsstrahlung x-rays.

2. GENERATOR

Figure 1 shows a block diagram of a compact monochromatic x-ray generator. This generator consists of the following components: a constant high-voltage power supply (SL150, Spellman Inc.), a DC filament power supply, a turbomolecular pump, and an x-ray tube. The structure of the x-ray tube is illustrated in Fig. 2. The x-ray tube is a demountable diode which is connected to the turbomolecular pump with a pressure of approximately 0.5 mPa and consists of the following major devices: a molybdenum rod target 3.0 mm in diameter, a tungsten hairpin cathode (filament), a focusing (Wehnelt) electrode, a polyethylene terephthalate x-ray window 0.25 mm in thickness, and a stainless-steel tube body. In the x-ray tube, the positive high voltage is applied to the anode (target) electrode, and the cathode is connected to the tube body (ground potential). In this experiment, the tube voltage applied was from 22 to 36 kV, and the tube current was regulated to within 100 μA by the filament temperature. The exposure time is controlled in order to obtain optimum x-ray intensity. The electron beams from the cathode are converged to the target by the focusing electrode, and x-rays are produced through the focusing electrode. Because bremsstrahlung rays are not emitted in the opposite direction to that of electron trajectory (Fig. 3), clean molybdenum $K\alpha$ rays can be produced using a 20- μm -thick zirconium filter.

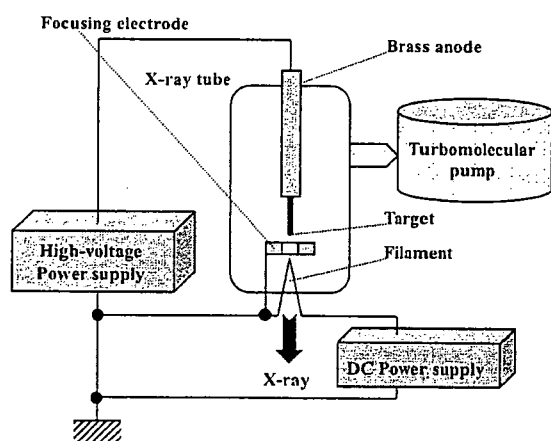


Figure 1: Block diagram including the main transmission line of the compact x-ray generator with a monochromatic diode.

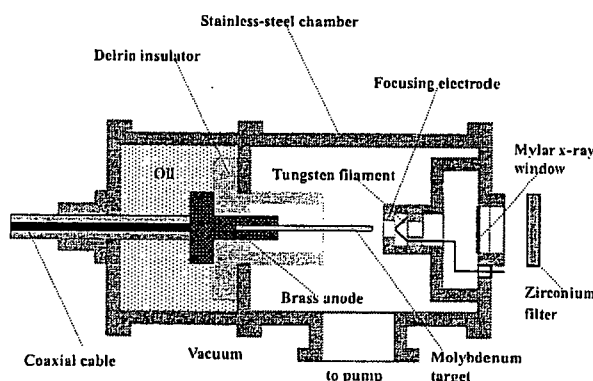


Figure 2: Schematic drawing of the monochromatic x-ray tube.

3. CHARACTERISTICS

3.1 X-ray intensity

X-ray intensity was measured by a Victoreen 660 ionization chamber at 1.0 m from the x-ray source (Fig. 4). At a constant tube current of 100 μA , the x-ray intensity increased when the tube voltage was increased. In this measurement, the intensity with a tube voltage of 30 kV and a current of 100 μA was 12.1 $\mu\text{Gy/s}$ at 1.0 m from the source.

3.2 X-ray source

In order to measure images of the x-ray source, we employed a pinhole camera with a hole diameter of 100 μm in conjunction with a computed radiography (CR) system¹⁸ (Fig. 5). When the tube voltage was increased, the spot diameter slightly increased and had a maximum value of approximately 2.3 mm.

3.3 X-ray spectra

X-ray spectra were measured using a transmission-type spectrometer with a lithium fluoride curved crystal 0.5 mm in thickness. The x-ray intensities of the spectra were detected by an imaging plate of the CR system (Konica Minolta Regius 150) with a wide dynamic range, and relative x-ray intensity was calculated from Dicom original digital data corresponding to x-ray intensity; the data was scanned by Dicom viewer in the film-less CR system. Subsequently, the relative x-ray intensity as a function of the data was calibrated using a conventional x-ray generator, and we confirmed that the intensity was proportional to the exposure time. Figure 6 shows measured spectra from the molybdenum target using the filter. We observed clean $K\alpha$ lines, while bremsstrahlung rays were hardly detected. The $K\alpha$ intensity substantially increased with increases in the tube voltage.

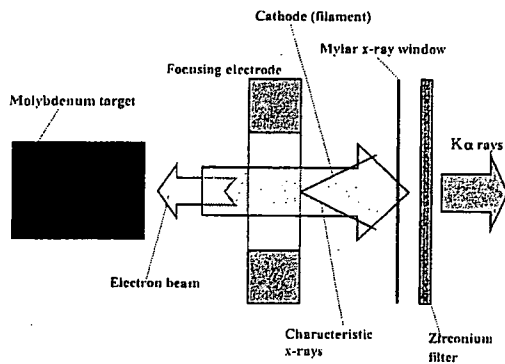


Figure 3: K-photon irradiation from the x-ray tube.

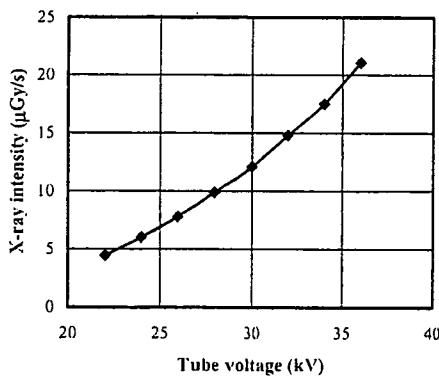


Figure 4: X-ray intensity at 1.0 m from the x-ray source according to changes in the tube voltage.

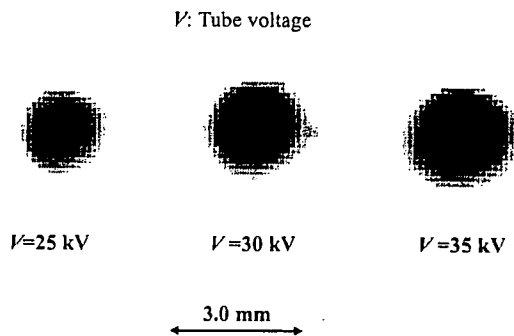


Figure 5: Images of the characteristic x-ray source obtained using a pinhole camera with changes in the tube voltage.

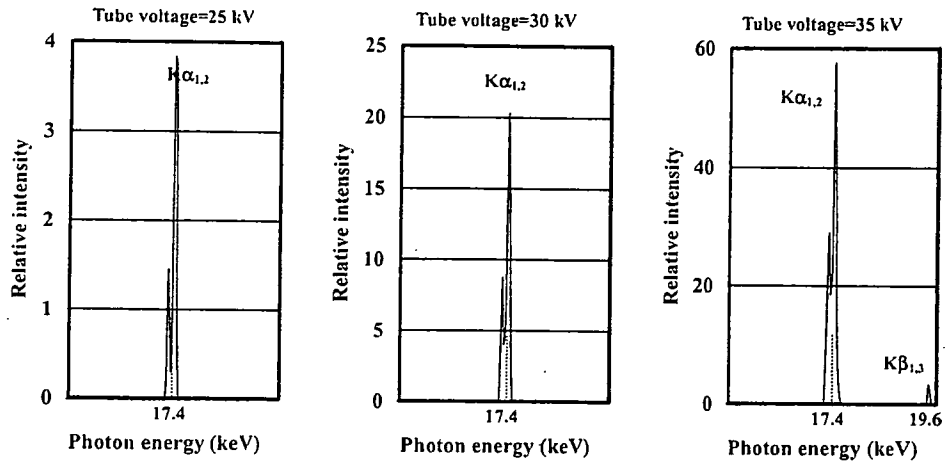



Figure 6: X-ray spectra from the molybdenum target. The spectra were measured using a transmission type spectrometer with a lithium fluoride curved crystal.

4. RADIOGRAPHY

The monochromatic radiography was performed by the CR system at 1.0 m from the x-ray source with the filter, and the tube voltage was 30 kV.

Firstly, rough measurements of image resolution were made using wires. Figure 7 shows radiograms of tungsten wires coiled around pipes made of polymethyl methacrylate (PMMA). Although the image contrast increased with increases in the wire diameter, a 50 μm -diameter wire could be observed.


A radiogram of a vertebra is shown in Fig. 8, and the fine structure of the vertebra was observed. Next, angiography was performed using iodine microspheres of 15 μm in diameter. Figures 9 and 10 show angiograms of a rabbit heart and thigh, respectively, and we could obtain high contrast images of coronary arteries and fine blood vessels.

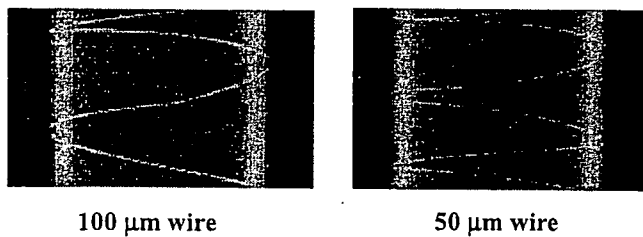

100 μm wire

50 μm wire

25 mm

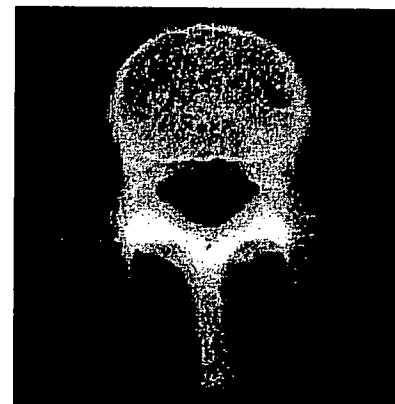

50 mm

Figure 7: Radiograms of tungsten wires of 50 and 100 μm in diameter coiled around pipes made of polymethyl methacrylate. A 50 μm -diameter wire could be observed.

Figure 8: Radiogram of a vertebra. Fine structure of the vertebra were visible.



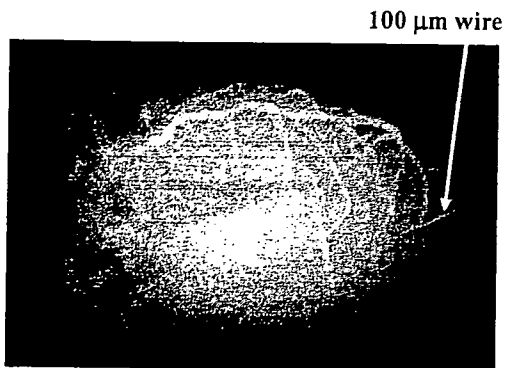


Figure 9: Angiograms of a rabbit heart. Coronary arteries were visible.

20 mm

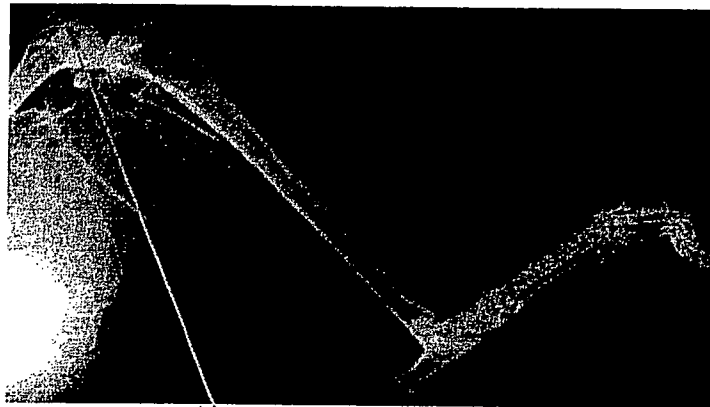

60 mm

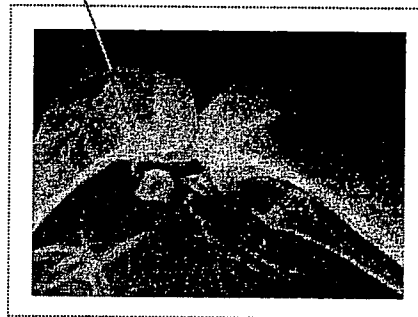

x2

Figure 10: Angiogram of a rabbit thigh. Fine blood vessels of approximately 100 μm in diameter were visible.

5. CONCLUSIONS AND OUTLOOK

We developed a new monochromatic x-ray generator with a molybdenum-target tube and succeeded in producing clean

molybdenum $K\alpha$ lines. The $K\alpha$ intensity increased with increases in the tube voltage, and monochromatic $K\alpha$ rays were left by the zirconium filter. Without using the filter, bremsstrahlung x-rays were hardly observed.

In this experiment, although the maximum tube voltage and current were 36 kV and 0.10 mA, the voltage and current could be increased to 100 kV and 1.0 mA, respectively. Under the pulsed operation, the current can be increased to approximately 1 A without considering the target evaporation. Subsequently, the maximum number of characteristic photons was approximately 5×10^6 photons/cm²·s at 1.0 m from the source, and the photon count rate can be increased easily by increasing the current.

The molybdenum K-series characteristic x-rays are useful for mammography, and the photon energies of characteristic x-rays can be selected by the target element. In particular, enhanced K-edge angiography can be performed using a cerium target because cerium $K\alpha$ rays (34.6 keV) are absorbed easily by iodine-based contrast media with an iodine K-edge of 33.2 keV. Furthermore, low-dose enhanced K-edge angiography can be performed utilizing a tungsten target in conjunction with gadolinium media.

Using these angiographies, coronary arteries and fine blood vessels formed in regenerative medicine may be observed with high contrasts. Furthermore, a flat panel detector is useful to observe blood flows for cases of cardiovascular disease.

ACKNOWLEDGMENTS

This work was supported by Grants-in-Aid for Scientific Research (13470154, 13877114, 16591181, and 16591222) and Advanced Medical Scientific Research from MECSSST, Health and Labor Sciences Research Grants (RAMT-nano-001, RHGTEFB-genome-005 and RHGTEFB-saisei-003), Grants from the Keiryō Research Foundation, The Promotion and Mutual Aid Corporation for Private Schools of Japan, Japan Science and Technology Agency (JST), and the New Energy and Industrial Technology Development Organization (NEDO, Industrial Technology Research Grant Program in '03).

REFERENCES

1. E. Sato, S. Kimura, S. Kawasaki, H. Isobe, K. Takahashi, Y. Tamakawa and T. Yanagisawa, "Repetitive flash x-ray generator utilizing a simple diode with a new type of energy-selective function," *Rev. Sci. Instrum.*, **61**, 2343-2348, 1990.
2. A. Shikoda, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa, "Repetitive flash x-ray generator having a high-durability diode driven by a two-cable-type line pulser," *Rev. Sci. Instrum.*, **65**, 850-856, 1994.
3. E. Sato, K. Takahashi, M. Sagae, S. Kimura, T. Oizumi, Y. Hayasi, Y. Tamakawa and T. Yanagisawa, "Sub-kilohertz flash x-ray generator utilizing a glass-enclosed cold-cathode triode," *Med. & Biol. Eng. & Comput.*, **32**, 289-294, 1994.
4. K. Takahashi, E. Sato, M. Sagae, T. Oizumi, Y. Tamakawa and T. Yanagisawa, "Fundamental study on a long-duration flash x-ray generator with a surface-discharge triode," *Jpn. J. Appl. Phys.*, **33**, 4146-4151, 1994.
5. E. Sato, M. Sagae, E. Tanaka, Y. Hayasi, R. Germer, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido: Quasi-monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube, *Jpn. J. Appl. Phys.*, **43**, 7324-7328, 2004.
6. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Compact monochromatic flash x-ray generator utilizing a disk-cathode molybdenum tube," *Med. Phys.*, **32**, 49-54, 2005.
7. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, H. Obara, T. Ichimaru, K. Takayama and H. Ido, "Irradiation of intense characteristic x-rays from weakly ionized linear molybdenum plasma," *Jpn. J. Med. Phys.*, **23**, 123-131, 2003.
8. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, K. Takayama and H. Ido, "Quasi-monochromatic flash x-ray generator utilizing weakly ionized linear copper plasma," *Rev. Sci. Instrum.*, **74**, 5236-5240, 2003.
9. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Sharp characteristic x-ray irradiation from weakly ionized linear plasma," *J. Electron Spectrosc. Related Phenom.*, **137-140**, 713-720, 2004.
10. E. Sato, E. Tanaka, H. Mori, T. Kawai, S. Sato and K. Takayama, "Clean monochromatic x-ray irradiation from weakly ionized linear copper plasma," *Opt. Eng.*, **44**, 049002-1-6, 2005.
11. E. Sato, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, H. Ojima, K. Takayama and H. Ido, "Quasi-monochromatic cerium flash angiography," *SPIE*, **5580**, 146-152, 2005.
12. T. J. Davis, D. Gao, T. E. Gureyev, A. W. Stevenson and S. W. Wilkins, "Phase-contrast imaging of weakly

absorbing materials using hard x-rays," *Nature*, **373**, 595-597, 1995.

13. A. Momose, T. Takeda, Y. Itai and K. Hirano, "Phase-contrast x-ray computed tomography for observing biological soft tissues," *Nature Medicine*, **2**, 473-475, 1996.

14. H. Mori, K. Hyodo, E. Tanaka, M. U. Mohammed, A. Yamakawa, Y. Shinozaki, H. Nakazawa, Y. Tanaka, T. Sekka, Y. Iwata, S. Honda, K. Umetani, H. Ueki, T. Yokoyama, K. Tanioka, M. Kubota, H. Hosaka, N. Ishizawa and M. Ando, "Small-vessel radiography in situ with monochromatic synchrotron radiation," *Radiology*, **201**, 173-177, 1996.

15. K. Hyodo, M. Ando, Y. Oku, S. Yamamoto, T. Takeda, Y. Itai, S. Ohtsuka, Y. Sugishita and J. Tada, "Development of a two-dimensional imaging system for clinical applications of intravenous coronary angiography using intense synchrotron radiation produced by a multipole wiggler," *J. Synchrotron Radiat.*, **5**, 1123-1126, 1998.

16. E. Sato, Y. Hayasi, R. Germer, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Portable x-ray generator utilizing a cerium-target radiation tube for angiography," *J. Electron Spectrosc. Related Phenom.*, **137-140**, 699-704, 2004.

17. E. Sato, E. Tanaka, H. Mori, T. Kawai, T. Ichimaru, S. Sato, K. Takayama and H. Ido, "Demonstration of enhanced K-edge angiography using a cerium target x-ray generator," *Med. Phys.*, **31**, 3017-3021, 2004.

18. E. Sato, K. Sato and Y. Tamakawa, "Film-less computed radiography system for high-speed imaging," *Ann. Rep. Iwate Med. Univ. Sch. Lib. Arts and Sci.*, **35**, 13-23, 2000.

*dresato@iwate-med.ac.jp; phone +81-19-651-5111; fax +81-19-654-9282

Energy-selective gadolinium angiography utilizing a stroboscopic x-ray generator

Eiichi Sato^{*a}, Yasuomi Hayasi^a, Rudolf Germer^b, Koji Kimura^c, Etsuro Tanaka^d, Hidezo Mori^e, Toshiaki Kawai^f, Takashi Inoue^g, Akira Ogawa^g, Shigehiro Sato^h, Kazuyoshi Takayamaⁱ and Hideaki Ido^j

^a Department of Physics, Iwate Medical University, 3-16-1 Honchodori, Morioka 020-0015, Japan

^b ITP, FHTW FB1 and TU-Berlin, Blankenhainer Str. 9, D 12249 Berlin, Germany

^c Department of Physiology, Tokai University School of Medicine, Boseidai, Isehara 259-1193, Japan

^d Department of Nutritional Science, Faculty of Applied Bio-science, Tokyo University of Agriculture, 1-1-1 Sakuragaoka, Setagaya-ku 156-8502, Japan

^e Department of Cardiac Physiology, National Cardiovascular Center Research Institute, 5-7-1 Fujishirodai, Suita, Osaka 565-8565 Japan

^f Electron Tube Division #2, Hamamatsu Photonics K. K., 314-5 Shimokanzo, Iwata 438-0193, Japan

^g Department of Neurosurgery, School of Medicine, Iwate Medical University, 19-1 Uchimarui, Morioka 020-8505, Japan

^h Department of Microbiology, School of Medicine, Iwate Medical University, 19-1 Uchimarui, Morioka 020-8505, Japan

ⁱ Shock Wave Research Center, Institute of Fluid Science, Tohoku University, 2-1-1 Katahira, Sendai 980-8577, Japan

^j Department of Applied Physics and Informatics, Faculty of Engineering, Tohoku Gakuin University, 1-13-1 Chuo, Tagajo 985-8537, Japan

ABSTRACT

Energy-selective high-speed radiography utilizing a kilohertz-range stroboscopic x-ray generator and its application to high-speed angiography are described. This generator consists of the following major components: a main controller, a condenser unit with a Cockcroft-Walton circuit, and an x-ray tube unit in conjunction with a grid controller. The main condenser of about 500 nF in the unit is charged up to 120 kV by the circuit, and the electric charges in the condenser are discharged to the triode by the grid control circuit. Although the tube voltage decreased during the discharging for generating x-rays, the maximum value was equal to the initial charging voltage of the main condenser. The maximum tube current and the repetition rate were approximately 0.5 A and 50 kHz, respectively. The x-ray pulse width ranged from 0.01 to 1.0 ms, and the maximum shot number had a value of 32. At a charging voltage of 100 kV and a width of 1.0 ms, the x-ray intensity obtained using a 50- μ m-thick tungsten filter was 9.88 μ Gy at 1.0 m, and the dimensions of the focal spot had values of approximately 1×1 mm. Angiography was performed using the filter at a charging voltage of 100 kV.

Keywords: energy-selective radiography, bremsstrahlung x-rays, filtering, stroboscopic x-ray, pulse x-ray, enhanced angiography

1. INTRODUCTION

Flash x-ray generators are capable of producing high-dose rate short x-ray pulses, and have been applied to high-speed radiography in various fields.¹ To produce hard flash x-rays with maximum photon energies of approximately 1 MeV, multistage Marx surge generators have been developed. Furthermore, induction linear accelerators have been developed

Ultrafast X-Ray Detectors, High-Speed Imaging, and Applications, edited by Stuart Kleinfelder, Dennis L. Paisley, Zenghu Chang, Jean-Claude Kieffer, Jerome B. Hastings, Proc. of SPIE Vol. 5920 (SPIE, Bellingham, WA, 2005) · 0277-786X/05/\$15 · doi: 10.1117/12.621056

Proc. of SPIE 59200V-1

and improved to produce 10-MeV-order flash x-rays.² In contrast, 100-kV-order flash x-ray generators have been developed and applied to biomedicine. Subsequently, soft x-ray lasers have been produced using a gas-discharge capillary,³⁻⁵ and clean K-series characteristic x-rays⁶⁻⁹ and their higher harmonic hard x-rays have been produced from weakly ionized linear plasma.

In high-speed medical radiography, the repetition rate is one of the technical key parameters in real-time dynamic radiography. In view of this situation, we have developed two stroboscopic x-ray generators¹⁰ and have succeeded in producing repetitive x-rays with a maximum repetition rate of approximately 50 kHz. These generators employ 500 nF condensers and hot-cathode tungsten tubes, and the duration can be controlled from 10 μ s to 1.0 ms

Recently synchrotrons generate monochromatic parallel x-ray beams using a monochromator, and these beams have been employed to perform enhanced K-edge angiography.¹¹⁻¹³ To perform angiography, the beams with photon energies of approximately 35 keV have been used, because iodine contrast media with a K-absorption edge of 33.2 keV absorb the beams effectively. In view of this situation, we have developed x-ray generators with cerium-target tubes^{14,15} which can produce $K\alpha$ rays (34.6 keV). Subsequently, we have performed energy-selective high-speed angiography¹⁶ using quasi-monochromatic x-rays produced by the aluminum filtering.

Gadolinium-based contrast media with a K-edge of 50.2 keV have been employed to perform angiography in MRI, and the gadolinium density has been increasing. In view of this situation, $K\alpha$ rays of tantalum (57.1 keV)¹⁷ and tungsten (58.9 keV) are also useful to perform angiography, because the $K\alpha$ rays are absorbed effectively by gadolinium media. As compared with angiography using iodine media, the absorbed dose can be decreased considerably utilizing angiography achieved with gadolinium media.

In this research, we employed a tungsten-target x-ray tube and performed a preliminary study on high-speed gadolinium angiography achieved with quasi-monochromatic x-rays produced by the tungsten filtering in conjunction with a computed radiography system.

2. GENERATOR

Figure 1 shows the block diagram of the kilohertz-range stroboscopic x-ray generator. This generator consists of the following major components: a main controller, a condenser unit with a Cockcroft-Walton circuit, and an x-ray tube unit in conjunction with a grid controller (Fig. 2). The main condenser of approximately 500 nF in the unit is charged up to 120 kV by the circuit, and the electric charges in the condenser are discharged to the triode by the grid control circuit. Although the tube voltage decreased during the discharging for generating x-rays, the maximum value was equal to the initial charging voltage of the main condenser. In this generator, positive and negative high voltages are applied to the anode and cathode electrodes, respectively.

The x-ray tube is a glass-enclosed hot-cathode triode and is composed of the following major parts: a rotating anode tube with a tungsten target, a focusing electrode, a hot cathode (filament), a grid, and a glass tube body. The electron beams from the cathode are accelerated between the anode and cathode electrodes and are converged to the target by the focusing electrode. The tube is set in the metal case filled with insulation oil, and the diaphragm regulates the irradiation field.

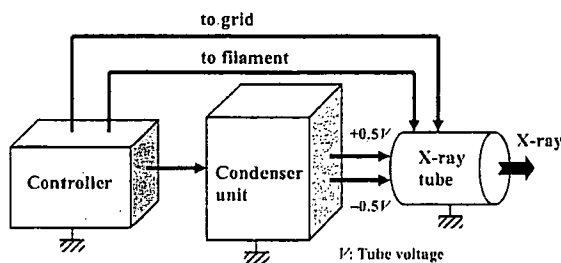


Figure 1: Block diagram of the kilohertz-range stroboscopic x-ray generator.

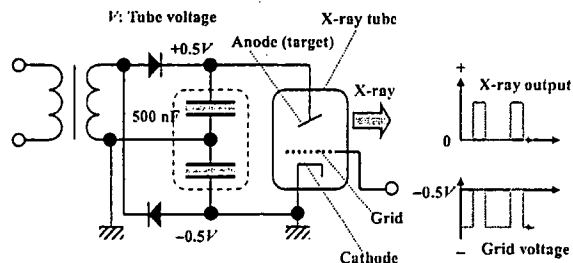


Figure 2: Main circuit of the kilohertz-range stroboscopic x-ray generator.