

Fig.4 Fluorescent images of albumin film on PVA hydrogel

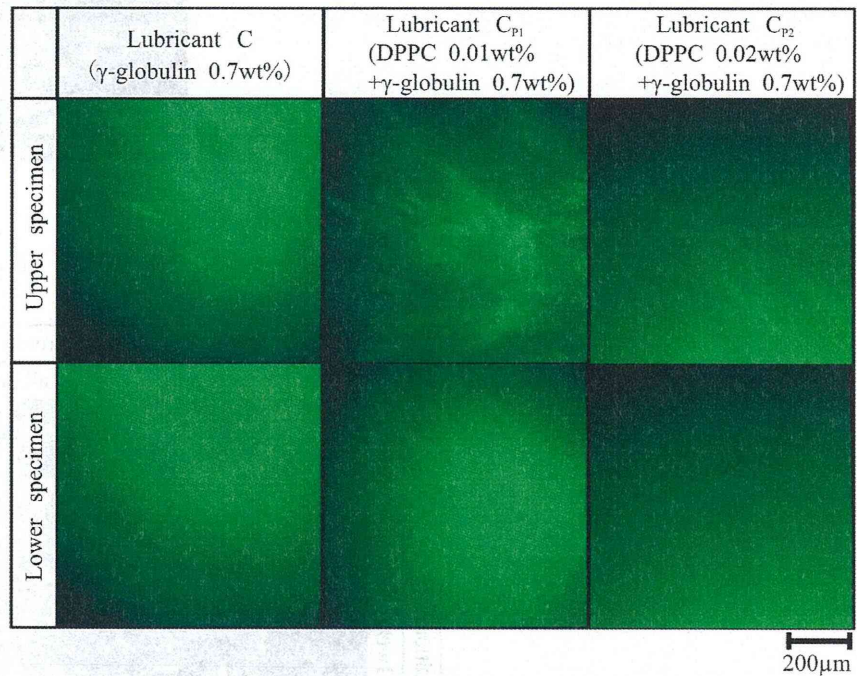


Fig.5 Fluorescent images of γ-globulin film on PVA hydrogel

The images of protein boundary film on PVA hydrogel by fluorescent observation were shown in Fig.4. Formation of smooth sheet-like adsorbed matters was observed in lubricant B_{P1} that contained 0.01wt% DPPC and albumin (Fig.4, arrows). However, degradation of forming sheet-like film was confirmed in lubricant B_{P2} that contained 0.02wt% DPPC. When lubricants contained γ-globulin as protein constituents, no sheet-like film was formed under coexistence of DPPC (Fig. 5).

Intact surface of PVA hydrogel and worn surfaces of PVA hydrogel as lower specimen were shown in Figs. 6 and 7, respectively. In normal saline, significant wear occurred with breaking off of the surface structure (Fig.7 (A)). In lubricant that contains albumin or

γ -globulin but no DPPC, severe wear occurred with loss of intact surface structure (Figs.7 (B), (C)). In lubricants that contain DPPC but no protein, severe abrasive wear occurred under low DPPC concentration and the reduction of wear was observed under high DPPC concentration (Fig.7 (A_{P2})). Wear reduction of PVA hydrogel was also confirmed in lubricant that contains protein and 0.01wt% DPPC (Figs. 3 (B_{P1}), (C_{P1})). However, both abrasive and adhesive wear patterns were observed in the lubricants that contains protein and 0.02wt% DPPC. These results indicated that DPPC contributes to reduction of friction and adhesivity and shifted the wear mode of PVA hydrogel from adhesive wear to abrasive wear. In addition, DPPC with high concentration and coexistence of DPPC with low concentration and protein reduce wear of PVA hydrogel. However, coexistence of DPPC with high concentration and protein has little effect in reducing wear of PVA hydrogel.

Worn surfaces of PVA hydrogel as upper specimen were shown in Fig.8. In lubricant A_{P1}, severe abrasive wear pattern with many scratches was confirmed. In contrast, significant wear occurred with breaking off of the surface structure in other lubricants. For all cases, there was no effect of lubricant additives on surface protection of PVA hydrogel as upper specimens.

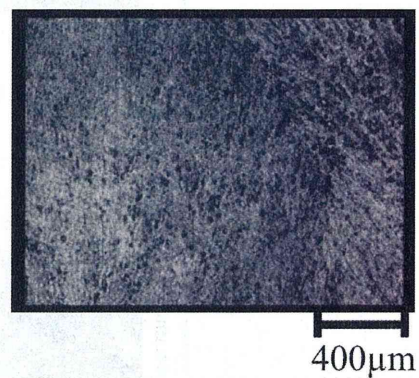


Fig.6 Intact surface of PVA hydrogel

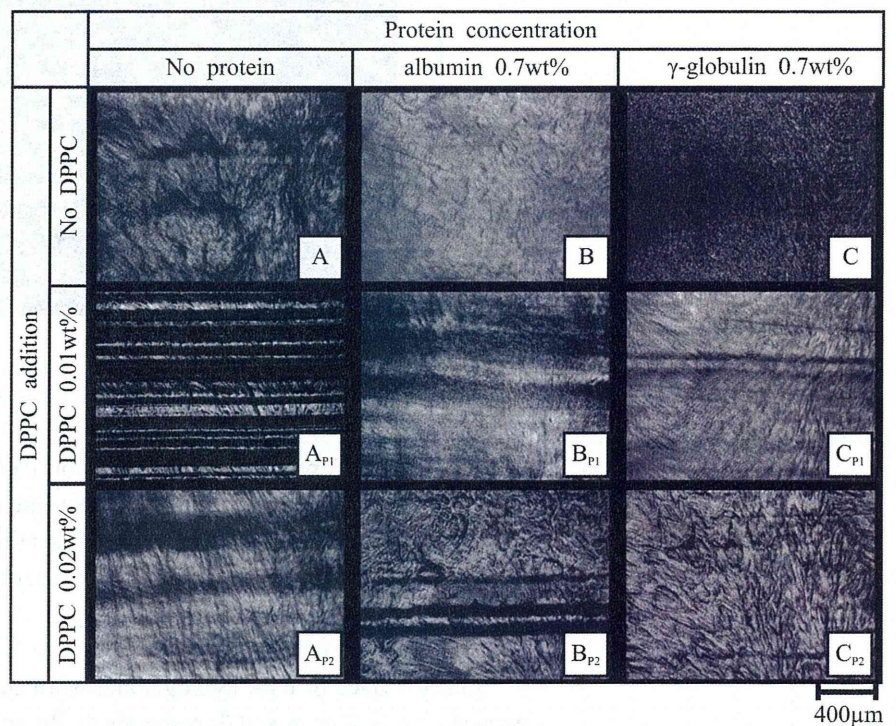


Fig.7 Worn surface of PVA hydrogel as lower specimens

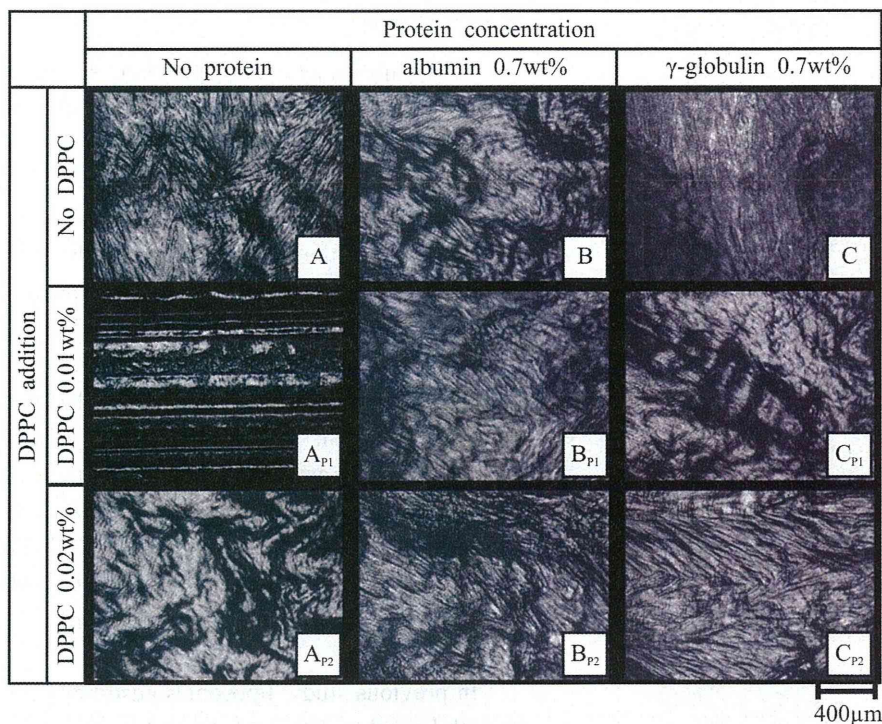


Fig.8 Worn surface of PVA hydrogel as upper specimens

3.2 TEM observation of lubricant components

TEM images of lubricant constituents are shown in Fig.9. Liposomes in lubricant A_{P1} are sized in several hundreds nanometers. In lubricant A_{P2} that contained twice as much DPPC as lubricant A_{P1}, some liposomes fused together and grew in size. When DPPC and proteins coexisted and concentration of DPPC was 0.01wt%, liposomes got distorted but remained their spherical structure. However, when the concentration of DPPC became higher as 0.02wt%, some liposomes aggregated and some lost their spherical structure and collapsed. Therefore, it was confirmed that DPPC/protein concentration in lubricant was key factor for the structure of liposomes and DPPC bilayers.

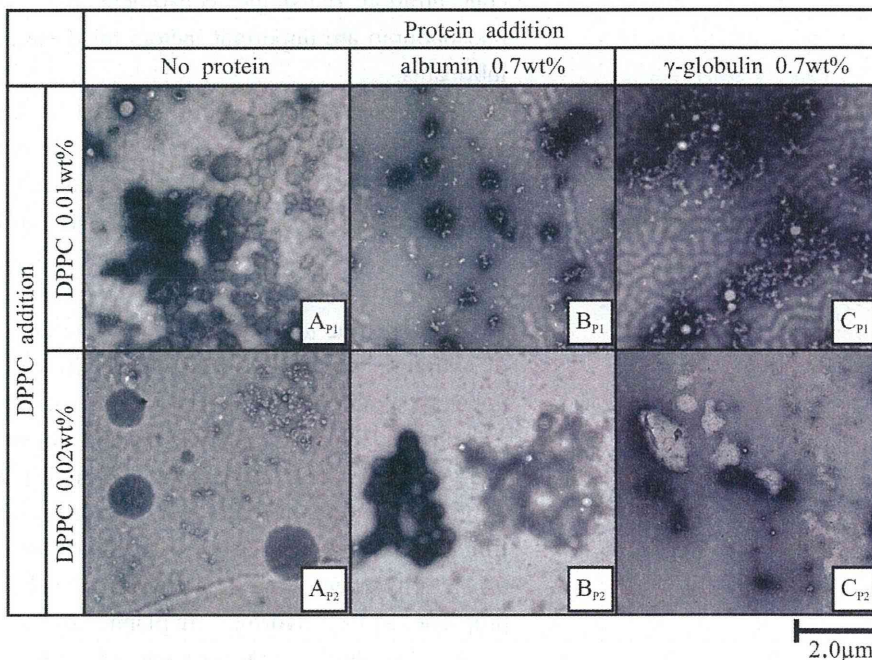


Fig.9 TEM images of lubricant components

4. Discussion

When lubricants contained DPPC but no proteins, friction coefficient was reduced by DPPC addition and wear pattern was shifted from adhesive to abrasive wear. In addition, wear of PVA hydrogel was suppressed by addition of DPPC with high concentration. Therefore, DPPC has role of reduction of the adhesivity and shear resistance between PVA hydrogels. The boundary lubricating ability of multi-lamellar film of phospholipids was reported⁽²⁸⁾, and the authors indicated the lubricating mechanisms of multi-lamellar film formed by friction-induced spread of liposomes⁽²⁴⁾. In lubricant that contained 0.01wt% DPPC, small liposomes easily collapsed and formed lamellar film based on the bilayer structure. In multi-lamellar film composed by phospholipid, water layer exists between each bilayer⁽²⁹⁾ and it is considered that this layer functions as a low shearing resistance layer. Although lubricant A_{P2} that contained 0.02wt% DPPC showed wear reduction of PVA hydrogel as compared to lubricant A_{P1} , there was little difference in friction coefficient at steady state between lubricants A_{P1} and A_{P2} . In general, liposomes are stabilized by fusion and enlargement. Therefore, wear of PVA hydrogel was reduced by increase of liposomes intervening between rubbing surfaces but additional effect of friction reduction was not obtained by suppression of forming multi-lamellar film due to the stabilization of liposomes.

In previous study, liposomes adsorbed on the rubbing surface were spread and formed smooth boundary film and showed low friction and the smooth sheet-like adsorbed matters that are composed of DPPC and albumin formed under rubbed condition⁽²⁴⁾. It was reported that the liposomes made by neutral phospholipids such as DPPC have high affinity to albumin⁽³⁰⁾ and there are influences of DPPC/protein concentration on maintaining and collapsing the structure of liposomes and phospholipid bilayers⁽³¹⁾. When concentration of liposomes in lubricant is low, the structures of liposomes and bilayers maintained and the liposomes did not become larger. And then, the liposomes were spread and formed lamellar film and functioned as boundary lubricant. When concentration of liposomes in lubricant is high, liposomes fused, grew in size and stabilized. Therefore, it is considered that liposomes in lubricants A_{P2} , B_{P2} , C_{P2} could not be easily spread by frictional loading and could not form multi-lamellar films. And thus, lubricating function of phospholipid was not fully utilized and adhesive wear pattern became obvious. These results indicated that not only concentration of single constituent but also relative concentration of proteins and phospholipid are important factors for these constituents to function as excellent boundary lubricants.

The effect of additives to lubricant on suppression of wear was not confirmed on the upper specimens. The contact area of upper specimens was not changed during reciprocating friction test. PVA hydrogel is the biphasic material that contains about 80% water and has biphasic lubrication property. It is indicated maintaining of water content and interstitial fluid pressure are important to maintaining the biphasic lubrication mechanism⁽³²⁾ and friction coefficient of PVA hydrogel as biphasic material increases with increase of loading time due to the exudation of internal water⁽³³⁾. There was little chance of recovery of hydration for upper specimen and it is considered that biphasic lubrication ability of upper specimens decreased during the test. Therefore, it is indicated that adsorbed film by proteins and phospholipid itself could not protect sufficiently the upper surface of PVA hydrogel with contact zone under continuous loading.

Thus, the establishment of the synergistic function of boundary lubrication by adsorbed film and biphasic lubrication is an important factor for reduction in both friction and wear of PVA hydrogel. The improvements in boundary lubrication and biphasic lubrication properties of PVA hydrogel are planned in further study.

In this study, concentration of proteins in lubricant was relatively low within

physiological concentration. In addition, natural synovial fluid contains other lubricating components such as hyaluronic acid. Therefore, influence of the addition of hyaluronic acid and protein concentration would be researched in future study.

5. Conclusion

In this study, influence of phospholipid and protein constituents on friction and wear behavior of PVA hydrogel as artificial cartilage was investigated. It was indicated that DPPC contributes to reduction of friction of PVA hydrogel and the appropriate coexistence of DPPC and proteins significantly reduces wear of PVA hydrogel. In addition, both the concentration and the relative ratio of proteins and phospholipids are important factors for these constituents to function as excellent boundary lubricants for PVA hydrogel. These findings would contribute to the elucidation of the wear mechanisms of PVA hydrogel in synovial fluid and improvement of material properties of PVA hydrogel considering the influences of synovial fluid as lubricants.

Acknowledgements

This research was supported by Grant-in-Aid for Specially Promoted Research of JSPS (23000011).


The authors would like to make a most cordial acknowledgment to Mr. T. Kanemaru in Kyushu University for his technical guidance on TEM observation and Mr. S. Hashimoto in Kyushu University for his effort in this research activity.

References

- (1) Willert, H.G., Semlitsch M. Reactions of the artificial capsule to wear products of artificial joint prostheses. *J Biomed Mater Res.*, Vol.11, No.2 (1977), pp.157-164.
- (2) Ingham, E., Fisher, J., Biological reactions to wear debris in total joint replacement. *Proc Inst Mech Eng Part H*, Vol.214, No.1 (2000), pp.21-37
- (3) McKellop, H., Shen, F.W., Lu, B., Campbell P, Salovey R. Development of an extremely wear-resistant ultra high molecular weight polyethylene for total hip replacements. *J. Orthop. Res.*, Vol.17, No.2 (1999), pp.157-167.
- (4) Oonishi, H., Kadoya, Y., Masuda, S., Gamma-irradiated cross-linked polyethylene in total hip replacements—analysis of retrieved sockets after long-term implantation, *J. Biomed. Mater. Res.*, Vol.58, No.2 (2001), pp.167-171.
- (5) Moro, T., Takatori, Y., Ishihara, K., Konno, T., Takigawa, Y., Matsushita, T., Chung, U.I., Nakamura, K., Kawaguchi, H., Surface grafting of artificial joints with a biocompatible polymer for preventing periprosthetic osteolysis, *Nat. Mater.* Vol.3, No.11 (2004), pp.829-836.
- (6) Jin, Z. M., Dowson, D., Fisher, J., Analysis of fluid film lubrication in artificial hip joint replacements with surfaces of high elastic modulus, *Proc. Instn. Mech. Engrs. Part H, Engineering in Medicine*, Vol.211, No.3 (1997), pp.247-256.
- (7) Ikeuchi, K., Ohashi, M., Tomita, N., Oka, M., The lubrication in ceramic-on-ceramic prostheses, *Jpn. J. Clin. Biomech.*, Vol.16 (1995), pp.381-383. (in Japanese)
- (8) Sasada, T., Takahashi, M., Watanabe, M., Mabuchi, K., Tsukamoto, Y., and Nanbu, M., Friction behavior of a total hip prosthesis containing artificial articular cartilage, *J. Jpn. Soc. Biomat.*, Vol.3, No.3 (1985), pp.151-157. (in Japanese)
- (9) Unsworth, A., Percy, M.J., White, E.F.T., White, G., Frictional properties of artificial hip joints, *Engng. Med.* Vol.17, No.3 (1988), pp.101-104.
- (10) Auger, D.D., Dowson, D., Fisher, J., Cushion form bearing for total knee joint

- replacement Part 1: design, friction and lubrication, *Proc. Inst. Mech. Engrs.*, Vol.209 (1995), pp.73-81.
- (11) Oka, M., Noguchi, T., Kumar, P., Ikeuchi, K., Yamamuro, T., Hyon, S.H., Ikada, Y., Development of an artificial articular cartilage, *Clin. Biomater.*, Vol.6 (1990), pp.361-381.
- (12) Murakami, T., Ohtsuki, N., Higaki, H., The adaptive multimode lubrication in knee prostheses with compliant layer during walking motion, *Thin Films in Tribology*, (1993), pp.673-682.
- (13) Murakami, T., Sawae, Y., Nakashima, K., Fisher, J., Tribological behaviour of artificial cartilage in thin film lubrication. *Thinning Films and Tribological Interfaces*, (2000), pp.317-327.
- (14) Mabuchi, K., Tsukamoto, Y., Yamamoto, M., Ueno, M., Sasada, T., Nambu, M., Lubrication property and mechanical durability of the joint prostheses containing cartilage-like polyvinyl alcohol gel, *J. Soc. Orthop. Biomech.*, Vol.8 (1986), pp.101-105. (in Japanese)
- (15) Shintani, H., Oka, M., Cha, W.I., Hyon, S.H., Ikada, Y., Ikeuchi, K., Sakaguchi, K., Hojo, H., Nakamura, T., The wear-resistant properties of PVA-hydrogel for artificial articular cartilage, *J. Jpn. Soc. Biomat.*, Vol.12, No.3 (1994), pp.127-134. (in Japanese)
- (16) Saikko, V., Ahlroos, T., Phospholipids as boundary lubricants in wear tests of prosthetic joint materials, *Wear*, Vol.207, Issues.1-2 (1997), pp.86-91.
- (17) Sawae, Y., Murakami, T., Chen, J., Effect of synovia constituents on friction and wear of ultra-high molecular weight polyethylene sliding against prosthetic joint materials, *Wear*, Vol.216 (1998), pp.213-219.
- (18) Namiki, O., Toyoshima, H., Morisaki, N., Therapeutic effect of intra-articular injection of high molecular weight hyaluronic acid on osteoarthritis of the knee, *Int. J. Clin. Pharmacol. Ther Toxicol.*, Vol. 20, Issue. 11 (1982), pp.501-507.
- (19) Kawano, T., Miura, H., Mawatari, T., Moro-Oka, T., Nakanishi, Y., Higaki, H., Iwamoto, Y., Mechanical effects of the intraarticular administration of high molecular weight hyaluronic acid plus phospholipid on synovial joint lubrication and prevention of articular cartilage degeneration in experimental osteoarthritis, *Arthritis Rheum.*, Vol.48, Issue 7 (2003), pp.1923-1929.
- (20) Hua, Z. K., Su, S. H., Zhang J. H., Tribological study on new therapeutic bionic lubricants, *Tribol. Lett.*, Vol.28, Issue 1 (2007), pp.51-58.
- (21) Nakashima, K., Murakami, T., Sawae, Y., Evaluation of wear property of PVA hydrogel as artificial cartilage and effect of protein film on wear-resistant property, *Trans. JSME Ser. C*, Vol.70, No.697 (2004), pp.2780-2787. (in Japanese).
- (22) Nakashima, K., Sawae, Y., Murakami, T., Study on wear reduction mechanisms of artificial cartilage by synergistic protein boundary film formation, *JSME Int. J. Ser C*, Vol.48, No.4 (2005), pp.555-561.
- (23) Yarimitsu, S., Nakashima, K., Sawae, Y., Murakami, T., Study on the mechanisms of wear reduction of artificial cartilage through in situ observation on forming protein boundary film, *Tribology Online*, Vol.2, No.4 (2007), pp.114-119.
- (24) Yarimitsu, S., Nakashima, K., Sawae, Y. and Murakami, T., Influences of synovia constituents on frictional behavior of artificial cartilage material and formation of boundary lubricating film, *J. Jpn. Soc. Tribol.*, Vol.55, No.7 (2010), pp.489-498. (in Japanese)
- (25) Rabinowitz, J. L., Gregg, J. R., Nixon, J. E., Lipid composition of the tissues of human knee joints. II. Synovial fluid in trauma, *Clin. Orthop. Relat. Res.*, Vol. 190 (1984), pp.292-298.

- (26) Mazzucco, D., Scott, R., Spector M., Composition of joint fluid in patients undergoing total knee replacement and revision arthroplasty: correlation with flow properties, *Biomaterials*, Vol.25, Issue 18 (2004), pp. 4433-4445.
- (27) Delecrin, J., Oka, M., Takahashi, A., Yamamuro, T., Nakamura T., Changes in joint fluid after total arthroplasty, *Clin. Orthop. Relat. Res.*, Vol.307 (1994), pp240-249.
- (28) Hills, B.A., Oligolamellar lubrication of joints by surface active phospholipids, *J. Rheum.*, vol.16, No.1 (1989), pp.82-91.
- (29) Pawlak, Z., Pao, R., Bayraktar, E., Kaldonski, T., Oloyede, A., Lamellar lubrication in vivo and vitro: Friction testing of hexagonal boron nitride, *Biosystems*, Vol.94, Iss.3 (2008), pp.202-208.
- (30) Hernandez-Caselles, T., Villalain, J., Gomez- Fernandez, J.C., Influence of liposome charge and composition on their interaction with human blood serum proteins, *Mol. Cell. Biochem.*, vol.120, No.2 (1993), pp.119-126.
- (31) Dimitrova, M. N., Matsumura, H., Protein-induced leakage and membrane destabilization of phosphatidylcholine and phosphatidylserine liposomes, *Colloids and Surfaces B: Biointerfaces*, Vol. 8 (1997), pp. 287-294.
- (32) Sakai, N., Hagihara, Y., Furusawa, T., Hosoda, N., Sawae, Y., Murakami, T., Analysis of biphasic lubrication of articular cartilage loaded by cylindrical indenter, *Tribol Intern.*, Vol.46, Iss.1 (2012), pp.225-236.
- (33) Murakami, T., Yarimitsu, S., Nakashima, K., Sawae, Y., Sakai, N., Adaptive multimode lubrication mechanism in articular cartilage and its application to artificial cartilage, *Proc. International Tribology Conference, Hiroshima 2011, USB memory (2011)*, G4-02.



An Additional Reference Axis Improves Femoral Rotation Alignment in Image-Free Computer Navigation Assisted Total Knee Arthroplasty

Hiroshi Inui MD, Shuji Taketomi MD, Kensuke Nakamura MD, Takaki Sanada MD, Sakae Tanaka MD, Takumi Nakagawa MD

Department of Orthopaedic Surgery, Faculty of Medicine, The University of Tokyo, Tokyo, Japan

ARTICLE INFO

Article history:

Received 17 August 2012

Accepted 28 January 2013

Keywords:

total knee arthroplasty
image-free navigation
femoral rotation
surgical transepicondylar axis
condylar twist angle

ABSTRACT

Few studies have demonstrated improvement in accuracy of rotational alignment using image-free navigation systems mainly due to the inconsistent registration of anatomical landmarks. We have used an image-free navigation for total knee arthroplasty, which adopts the average algorithm between two reference axes (transepicondylar axis and axis perpendicular to the Whiteside axis) for femoral component rotation control. We hypothesized that addition of another axis (condylar twisting axis measured on a preoperative radiograph) would improve the accuracy. One group using the average algorithm (double-axis group) was compared with the other group using another axis to confirm the accuracy of the average algorithm (triple-axis group). Femoral components were more accurately implanted for rotational alignment in the triple-axis group (ideal: triple-axis group 100%, double-axis group 82%, $P < 0.05$).

© 2013 Elsevier Inc. All rights reserved.

Total knee arthroplasty (TKA) has become one of the most successful surgical procedures in orthopedic surgery [1,2]. The success of this procedure depends on many factors, including surgical techniques and the design and material of the components. With regard to surgical techniques, implant positioning and soft tissue balancing are very important. Malpositioning of any component can lead to an increased risk of loosening, instability, patella subluxation, and residual pain [3–5].

Computer-assisted navigation systems have been designed to increase the accuracy of implantation and have become much more accepted and prevalent in recent years. Several studies have demonstrated superior alignment of components in the coronal plane in navigated TKA compared with conventionally implanted TKA [6–8]. However, with regard to the accuracy of rotational alignment, few studies have demonstrated an improvement in computer-assisted navigation as compared with conventional methods. In particular, using image-free navigation systems, many authors have reported variability in identifying the surgical transepicondylar axis (SEA) for femoral rotation [9–11]. The Whiteside axis is generally assumed to be perpendicular to SEA and therefore a reliable axis of reference [12,13]. However, criticism of this landmark also includes difficulty in identification in case of trochlear dysplasia or destructive arthritis [14,15]. Using an average algorithm between

the determined angle of the registered Whiteside axis and transepicondylar axis has been recommended, and Stockl et al. showed that image-free navigation using this algorithm improved femoral rotational alignment [15,16]. However, much room for improvement in femoral component rotation control remains in the use of image-free navigation systems.

To reduce the registration errors, we believed that there is a need for an additional reference axis to confirm the accuracy of the rotational axis calculated by the image-free navigation system using an average algorithm. If the additional axis contradicts the rotational axis calculated by the image-free navigation system, it shows the necessity to re-register such landmarks as the medial sulcus, lateral epicondyle, and femoral AP axis. The posterior condylar axis (PCA) is known to be one of the most common axes during conventional total knee arthroplasty procedure. However, there are differences among patients in the angle between SEA and PCA, which is often called the condylar twist angle (CTA); therefore, CTA must be measured preoperatively to accurately set the rotational cutting guide in the conventional technique. Indeed, the use of computed tomography (CT) or magnetic resonance imaging (MRI) is recommended to detect CTA, but this accompanies some disadvantages, including the additional cost of CT and MRI and the additional radiation dose associated with CT. However, there have been some reports on methods that can help us to predict PCA and CTA preoperatively from radiography alone [17–19]. Just one additional radiograph is less of a disadvantage than CT or MRI.

The purpose of this study was to clarify whether the accuracy of the femoral rotational axis derived from an image-free navigation

The Conflict of Interest statement associated with this article can be found at <http://dx.doi.org/10.1016/j.arth.2013.01.030>.

Reprint requests: Hiroshi Inui, MD, Department of Orthopaedic Surgery, Faculty of Medicine, The University of Tokyo, 7-3-1 Hongo, Bunkyo-ku, Tokyo 113-0033, Japan.

system using an average algorithm could be confirmed by calculating another reference axis determined by PCA and CTA predicted from one additional radiograph, and also whether this improved femoral rotational alignment. We therefore hypothesized that this confirmation using the additional axis would improve femoral rotational alignment.

Materials and Methods

Institutional review board approval was received for this study. All patients provided written informed consent.

Of a total of 162 consecutive primary TKA procedures performed in 146 patients between January 2009 and September 2011, 158 knees were replaced using the Stryker 4.0 image-free computer navigation system (Stryker Orthopedics, Mahwah, NJ) equipped with an average algorithm derived from the registered Whiteside axis and SEA.

Between January 2009 and June 2010, femoral rotational alignment was determined according to this navigation algorithm (double-axis group: 78 knees) and between July 2010 and September 2011, femoral rotational alignment was determined by the navigation system and confirmed by the additional axis (triple-axis group: 80 knees). With power set at 0.80 and a 2-sided P-value of 0.05, we calculated 24 patients would be needed in each group to detect the accuracy of the femoral rotational alignment. Thirty-eight knees in the double-axis group and 26 knees in the triple-axis group were assessed by axial CT imaging after surgery. Preoperative variables were recorded, including age, sex, body mass index, preoperative diagnosis, frontal alignment, and range of motion. Pre-operative scores were obtained using the Knee Society Score (KSS) [20]. There was no statistically significant difference between the groups in terms of demographic characteristics (Table 1).

Pre-Operative Planning

Preoperatively, in the triple-axis group, one radiograph of the distal femur was taken by the method of Kanekasu et al. [17], and we contrived to see the epicondyles and posterior condyles of the femur by radiography as accurately as by axial CT imaging. We measured the angle between the clinical epicondylar axis (CEA) and PCA on the radiograph (Fig. 1). Then, we considered the influences of two things. One was the angle between CEA and SEA which had been reported to be 3° [18]. The other was the residual articular cartilage of the posterior condyle which the radiograph was unable to detect (Fig. 2). Takashiro et al. [19] demonstrated that the articular cartilage wear of the posterior femoral condyle affected CTA and that the articular cartilage wear of the posterior femoral condyle of patients with varus knees was mainly localized in the posteromedial condyle. We assumed that the cartilage wear would be localized in the posterolateral condyle of patients with valgus knees and the cartilage wear of the posteromedial and posterolateral condyle of patients with neutral knees would be equal, and that the angle affected by the cartilage wear was 1° [19]. Therefore, we subtracted 4° (=3° + 1°) from the measured angle for varus knees,

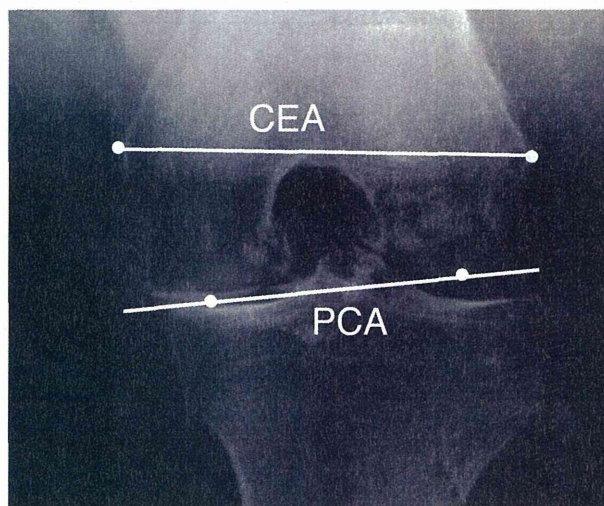


Fig. 1. Axial radiograph of the distal femur taken by the method of Kanekasu et al. [17]. CEA is the line connecting the medial and lateral epicondylar prominences; PCA is the line connecting the posterior margins of the medial and lateral femoral condyles.

3° for neutral knees, and 2° (=3°–1°) for valgus knees in this study to attain the predicted condylar twist angle (p-CTA) (Fig. 2). The average p-CTA was 3.7° ± 1.0° of external rotation [mean ± standard deviation (SD), range: 1°–7° of external rotation].

Surgical Procedure

The Stryker 4.0 Navigation System was used for computer-assisted implantation. The system was image-free and used infrared cameras and light-emitting diodes. Surgery was performed under a tourniquet. A midvastus approach was used for varus and neutral knees and a medial parapatellar approach was used for valgus knees. The patella was everted in all patients. Landmarks comprised the center of the femoral head, the distal femur, the proximal tibia, the ankle, the Whiteside axis, the epicondylar axis (lateral epicondyle, medial sulcus), the anterior surface of the distal femoral cortex, the condylar surfaces of the femur and tibia, and the tibial AP axis. The femoral rotation axis on the navigation system (navi-FRA) was defined as the average rotational axis of the transepicondylar axis and the axis perpendicular to the Whiteside axis in the double-axis group (Fig. 3).

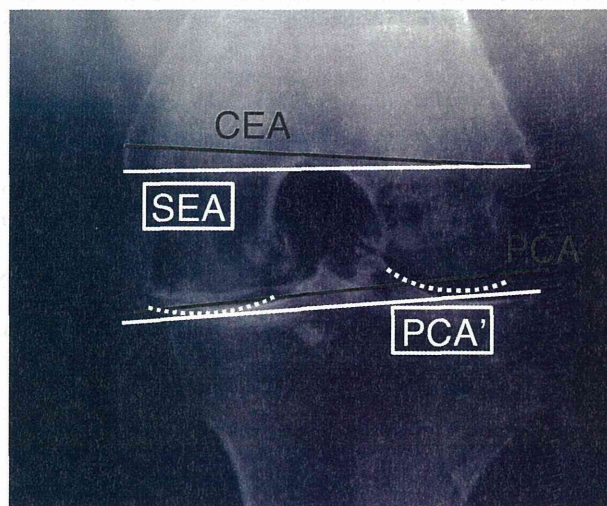


Fig. 2. Predicted condylar twist angle (p-CTA). P-CTA is the angle between SEA and PCA'. PCA' is the line connecting the posterior margins of the two dotted curves which are the assumed posterior femoral condyles with the articular cartilage included.

Table 1
Preoperative Demographic Data.

	Double-Axis Group	Triple-Axis Group	P-Value
Number of patients	38	26	
Sex (female/male)	32/6	21/5	
Diagnosis (OA/AN)	36/2	24/2	
Age (years)	76.8 ± 4.6	79.6 ± 5.1	n.s.
Pre-operative FTA (°)	185.6 ± 9.6	186.5 ± 6.0	n.s.
Pre-operative KSS	36.4 ± 10.1	34.9 ± 9.7	n.s.
Maximum extension (°)	–10.9 ± 6.7	–9.4 ± 6.1	n.s.
Maximum flexion (°)	120.3 ± 14.2	120.0 ± 11.8	n.s.
Body mass index (kg/m ²)	25.6 ± 3.9	25.2 ± 3.5	n.s.

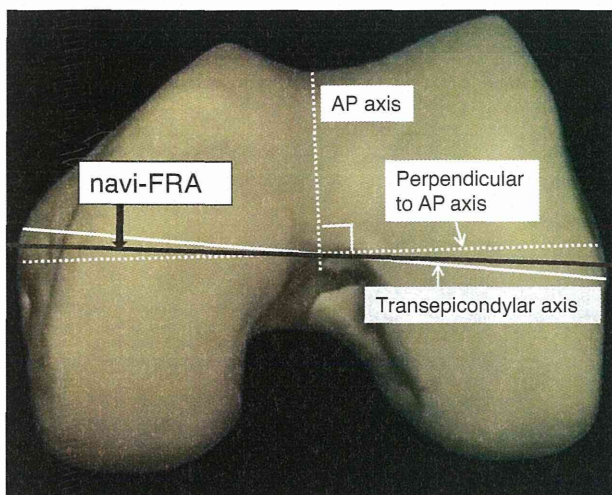


Fig. 3. The femoral rotation axis on the navigation system (“navi-FRA”). Navi-FRA is defined as the average axis of the transepicondylar axis and the axis perpendicular to the AP axis. AP axis = Whiteside’s line.

In the triple-axis group, after cutting the distal femur, the posterior reference guide was set. Using the posterior reference guide, we drew two blue lines, one of which was “p-CTA -2° ” externally rotated from PCA and the other was the “p-CTA $+2^\circ$ ” externally rotated (Fig. 4). We measured the angles between navi-FRA and the two lines intraoperatively using the navigation template drilling guide. The guide was one of the specific adapted instruments of the Stryker 4.0 system which was developed to calculate the angle between PCA and the line connecting two drill holes or between PCA and the lower end of the guide (Fig 5). If the former angle was displayed as “internal” and the latter as “external,” we concluded that navi-FRA was set as accurately as possible since the differences between navi-FRA and the axis determined by PCA and p-CTA were within 2° (Fig. 5). If both angles were displayed as internal or external, we assumed that the registration had not been performed accurately, and we re-registered the three landmarks (lateral epicondyle, medial sulcus, and the Whiteside axis). After one more registration, we followed navi-FRA and set the 4-in-1 cutting block.

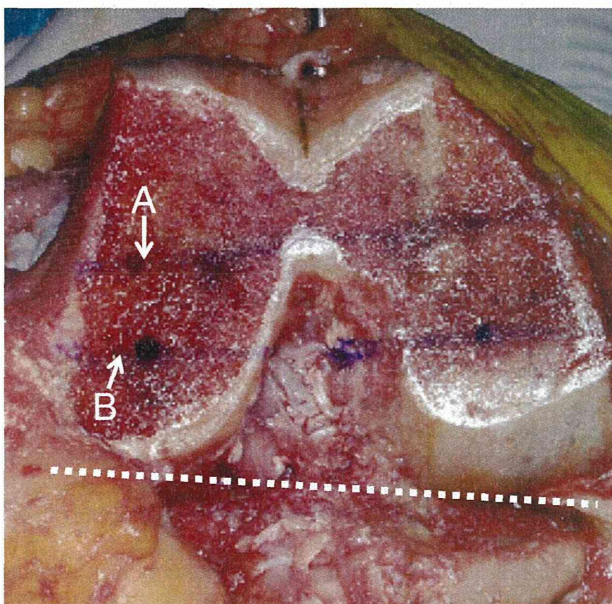


Fig. 4. Axial cross-section of the right distal femur. A: a blue line “p-CTA $+2^\circ$ ” externally rotated from PCA. B: a blue line “p-CTA -2° ” externally rotated from the PCA. PCA is the dotted line in this figure.

One surgeon (TN) took part in all procedures as the chief surgeon or first assistant. All implants used in both groups were Stryker Scopio NRG total knee implants.

Postoperative Evaluation

Rotational alignment of the femoral component was evaluated by CT. Knees were positioned in full extension. The rotational femoral component (RFC) angle was defined as the angle between the line through the center of both fixation pegs and SEA (Fig. 6). The ideal rotational femoral component angle was defined as falling within 3° of the target angle (0°) [9]. All CT scans were measured twice at 3-month intervals by two observers (HI and TS). Postoperative scores (KSS) and range of motion were recorded 1 year after operation.

Statistical Analysis

Data were analyzed using the EXCEL statistics 2008 (SSRI Co., LTD., Tokyo, Japan) software package for Microsoft Windows. The Mann-Whitney U-test was used to compare the two groups. Fisher’s exact probability test was used to compare the rate of optimally implanted components between the two groups. All significance tests were two-tailed, and a significance level of $P < 0.05$ was used for all tests. The chance-corrected κ -coefficient was calculated to determine the intra- and inter-observer agreements. Kappa values of intra-observer reliability, inter-observer reliability (HI), and inter-observer reliability (TS) were 0.84, 0.91, and 0.92, respectively.

Results

The average RFC angle was $-0.1^\circ \pm 2.4^\circ$ [mean \pm SD, range: 7° of internal rotation to 4° of external rotation] for the double-axis group and $0.3^\circ \pm 1.7^\circ$ (3° of external rotation to 3° of internal rotation) for the triple-axis group. With regard to the average RFC angle, there were no statistically significant differences observed between the two groups.

Thirty-one cases (82%) were implanted ideally (within 3° of neutral) in the double-axis group, whereas all 26 cases (100%) were implanted ideally in the triple-axis group. There was a statistically significant improvement in the triple-axis group ($P < 0.05$) (Fig. 7).

In the triple-axis group, a second registration was necessary for 8 cases (31%). After re-registration, navi-FRA was set accurately in all cases. There were 2 cases in which both of the angles between navi-FRA and the two blue lines after the second registration were displayed as internal and one case in which they were external.

The mean post-operative KSS was 91.7 (range: 79 to 100) for the double-axis group and 93.5 (75 to 100) for triple-axis group. The mean post-operative functional score was 72.2 (5 to 100) for the double-axis group and 74.7 (30 to 100) for triple-axis group. With regard to range of motion, the average maximum extension angle and flexion angle were -2.1° (-20° to 5°) and 115.8° (90° to 135°) for the double axis group, while -1.8° (-10° to 5°) and 118.2° (95° to 135°) for the triple-axis group. No significant difference was detected in these values for the two groups. There was one case of patella subluxation in the double-axis group which needed an additional operation of arthroscopic lateral release, the femoral component of which was 6° internally implanted.

Discussion

Malpositioning of any component can lead to an increased risk of loosening, instability, and pain [3,4]. Restoration of the tibiofemoral angle to within 3° of neutral during TKA is thought to be associated with a better outcome [4–6,21,22]. Computer-assisted navigation systems are designed to increase the accuracy of implantation, and have become much more accepted and prevalent in recent years.